

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
 Data File : BN005266.D
 Acq On : 25 Apr 2019 00:31
 Operator : JU/SJ
 Sample : K2456-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHP6

Quant Time: Apr 25 04:19:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	275673	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1245480	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	778814	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	1726330	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	1211171	20.00	ng/ul	-0.02
85) Perylene-d12	23.41	264	1223602	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	49521	8.67	ng/uL	0.00
5) Phenol-d5	6.78	99	1126771	52.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	691090	51.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	888741	53.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	950552	56.16	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	484372	63.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	538615	69.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	999990	56.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1396557	76.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3271075	57.86	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3987187	57.42	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	487836	54.65	ng/ul	0.00
57) Fluorene-d10	15.23	176	2744086	57.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	324073	41.74	ng/ul	0.00
70) Anthracene-d10	17.08	188	4132309	57.10	ng/ul	0.00
78) Pyrene-d10	19.39	212	4139224	66.81	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	3167266	59.23	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	828915	14.715	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
Data File : BN005266.D
Acq On : 25 Apr 2019 00:31
Operator : JU/SJ
Sample : K2456-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHP6

Quant Time: Apr 25 04:19:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

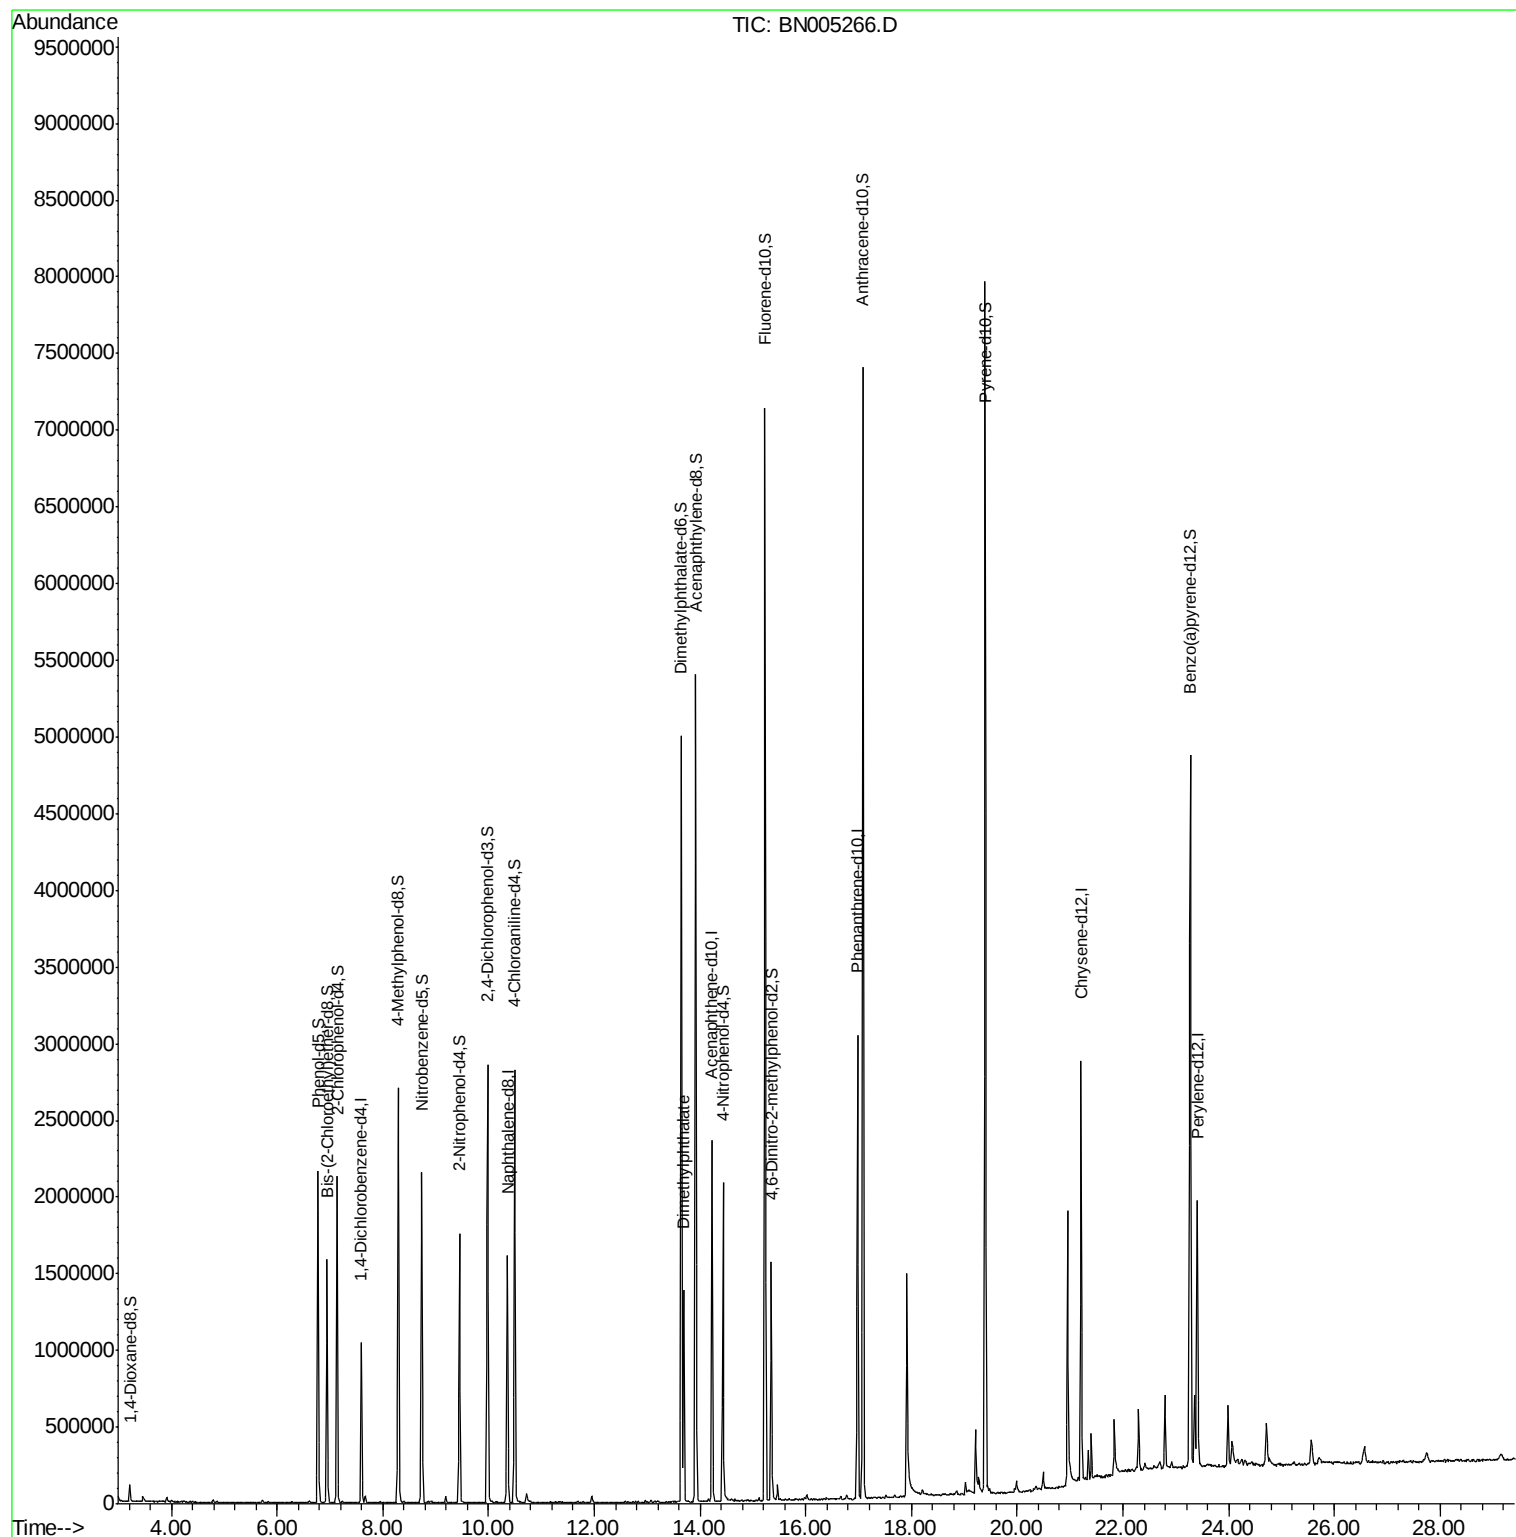

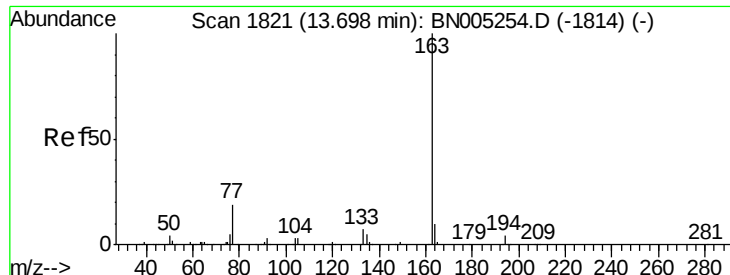

#44
 Dimethylphthalate
 Concen: 14.715 ng/ul
 RT: 13.69 min Scan# 1820
 Delta R.T. -0.01 min
 Lab File: BN005266.D
 Acq: 25 Apr 2019 00:31

Instrument :
 BNA_N
 ClientSampleId :
 GAHP6

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.0
164	10.5	8.1	12.1

