

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
 Data File : BN005281.D
 Acq On : 25 Apr 2019 09:44
 Operator : JU/SJ
 Sample : K2456-22
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GAHP0

Quant Time: Apr 25 10:27:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	438433	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1968286	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1212720	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2738078	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	2098226	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2014797	20.00	ng/ul	-0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	44885	4.94	ng/uL	0.00
5) Phenol-d5	6.78	99	1060500	30.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	619426	28.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	831955	31.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	890099	33.07	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	441293	36.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	499918	40.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	924444	32.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1282432	44.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3022319	34.33	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	3684247	34.07	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	465681	33.50	ng/ul	0.00
57) Fluorene-d10	15.23	176	2561882	34.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	324423	26.34	ng/ul	0.00
70) Anthracene-d10	17.08	188	3974419	34.63	ng/ul	0.00
78) Pyrene-d10	19.39	212	4173690	38.88	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	3140085	35.66	ng/ul	-0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	856903	9.769	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
Data File : BN005281.D
Acq On : 25 Apr 2019 09:44
Operator : JU/SJ
Sample : K2456-22
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GAHP0

Quant Time: Apr 25 10:27:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

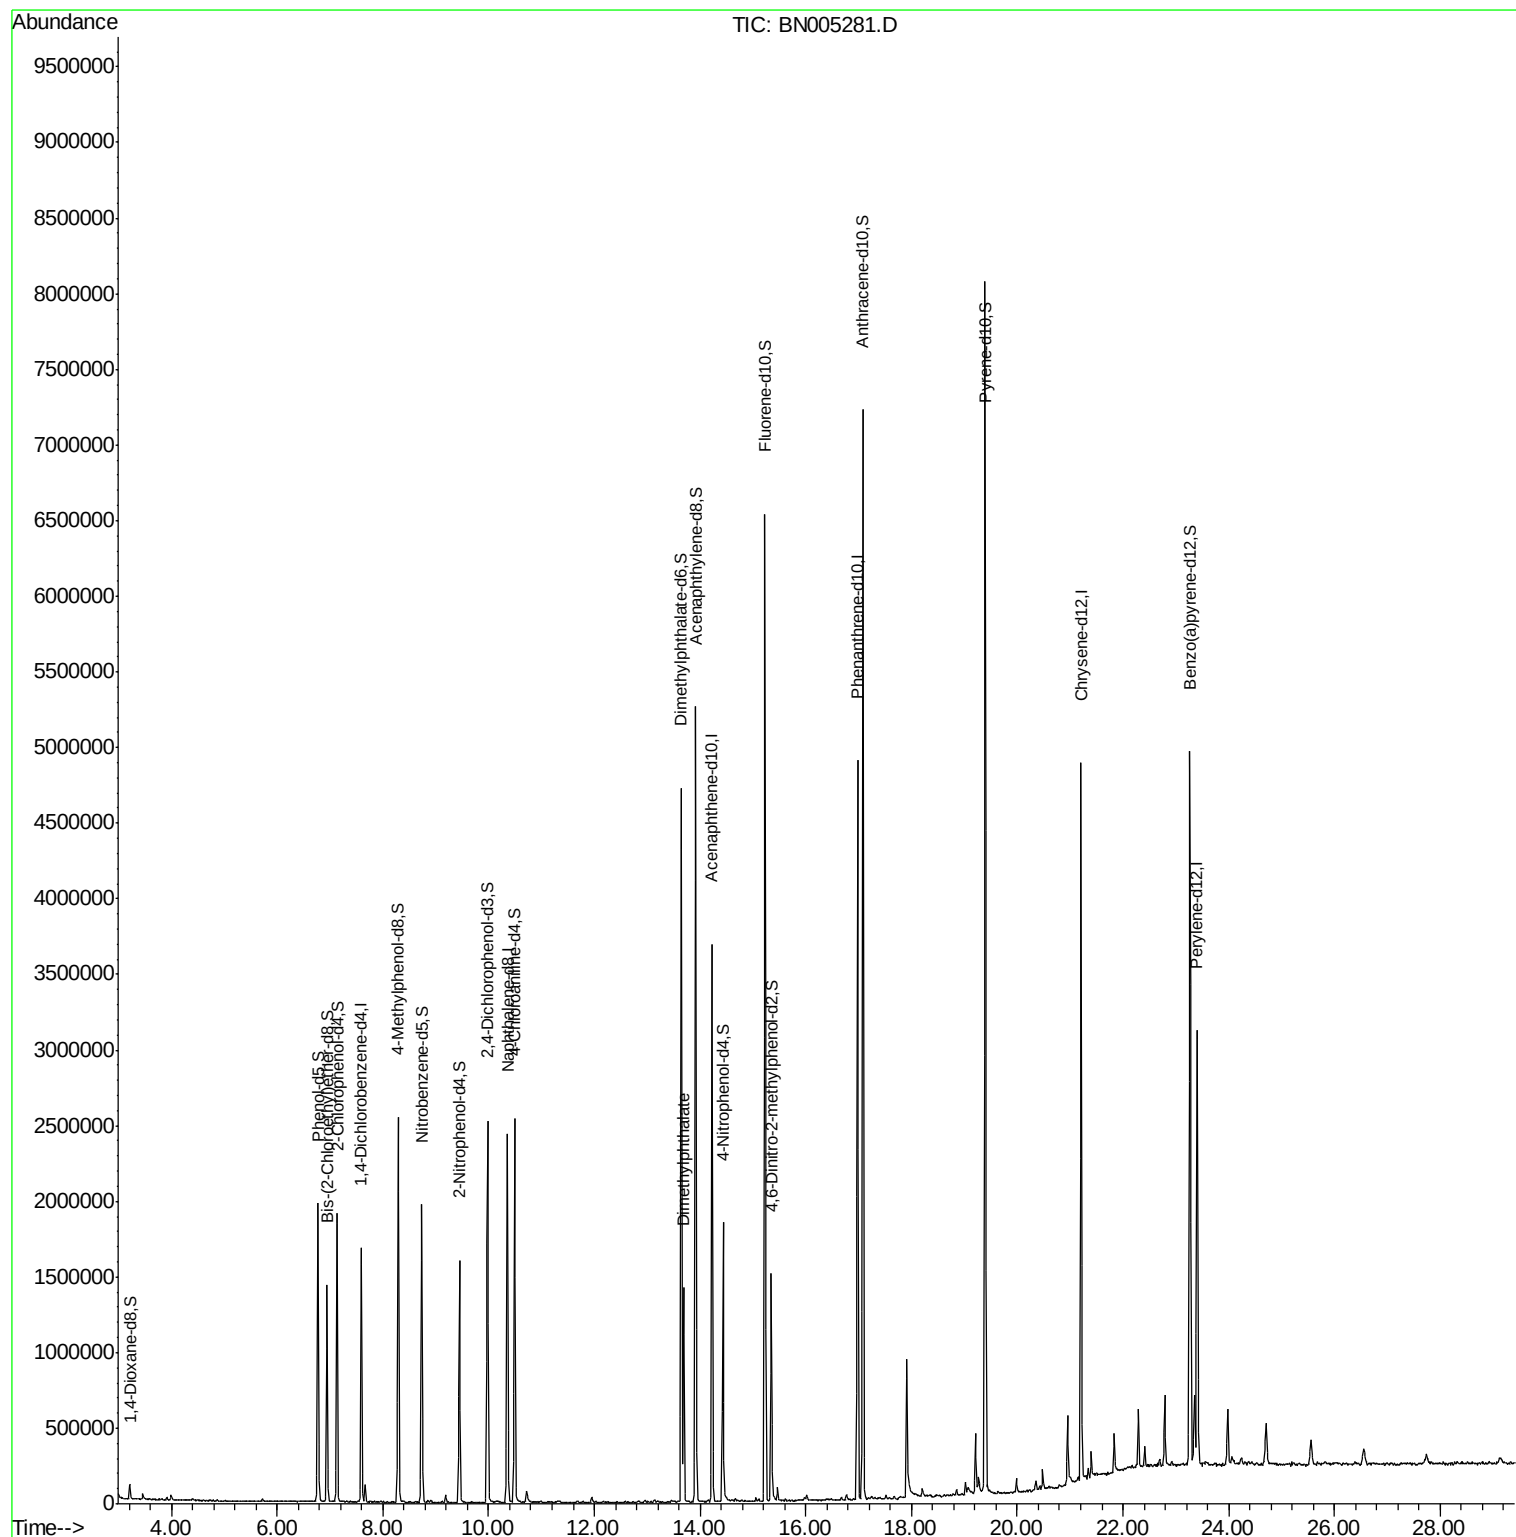

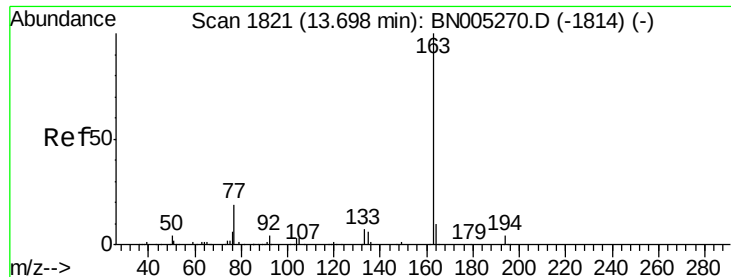

#44

Dimethylphthalate

Concen: 9.769 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005281.D

Acq: 25 Apr 2019 09:44

Instrument :

BNA_N

ClientSampleId :

GAHP0


Tot Ion:163 Resp: 856903

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.4 8.1 12.1

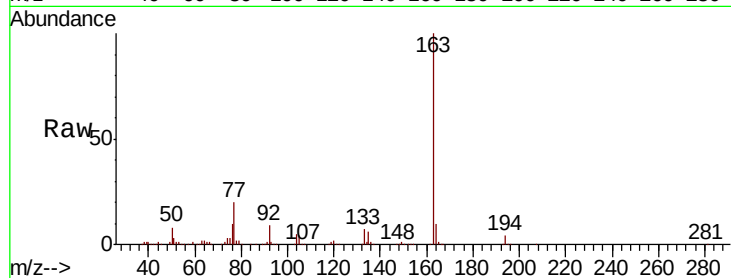

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

