

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
 Data File : BN005255.D
 Acq On : 24 Apr 2019 18:08
 Operator : JU/SJ
 Sample : PB119036BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK36

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	47	rVB	66027	82835	1.45%	0.120%
2	3.911	153	157	161	rBV3	13540	19435	0.34%	0.028%
3	4.870	317	320	323	rVB4	5692	6048	0.11%	0.009%
4	6.775	636	644	655	rBV	1077977	1648468	28.93%	2.390%
5	6.946	667	673	685	rVB	771938	1229709	21.58%	1.783%
6	7.134	697	705	714	rBV	1048915	1649521	28.95%	2.392%
7	7.593	777	783	793	rVB	1482941	2411670	42.32%	3.497%
8	8.034	852	858	860	rBV2	3537	5745	0.10%	0.008%
9	8.293	894	902	913	rBV	1330337	2086472	36.61%	3.025%
10	8.411	916	922	924	rBV6	4490	7267	0.13%	0.011%
11	8.734	968	977	990	rBV	1051488	1667636	29.26%	2.418%
12	9.446	1091	1098	1109	rBV	773379	1315328	23.08%	1.907%
13	9.981	1181	1189	1200	rBV	1336898	2227447	39.09%	3.230%
14	10.357	1246	1253	1263	rBV	2258275	3698995	64.91%	5.363%
15	10.493	1269	1276	1287	rBV	1333482	2274318	39.91%	3.298%
16	11.957	1519	1525	1531	rBV3	15099	30983	0.54%	0.045%
17	13.187	1731	1734	1741	rVB3	4720	9846	0.17%	0.014%
18	13.598	1799	1804	1806	rBV2	4750	6545	0.11%	0.009%
19	13.646	1806	1812	1826	rVB	2331200	3297950	57.87%	4.782%
20	13.916	1851	1858	1869	rBV	2731185	3924715	68.87%	5.691%
21	14.228	1904	1911	1920	rBV2	3186829	5029882	88.26%	7.293%
22	14.287	1920	1921	1928	rVB4	5866	8859	0.16%	0.013%
23	14.428	1939	1945	1963	rBV	705312	1239459	21.75%	1.797%
24	15.063	2048	2053	2056	rBV5	5164	8725	0.15%	0.013%
25	15.228	2074	2081	2088	rBV	3283036	4754228	83.43%	6.894%
26	15.351	2096	2102	2111	rBV	391892	588895	10.33%	0.854%
27	15.469	2116	2122	2128	rBV2	39017	65512	1.15%	0.095%
28	16.016	2209	2215	2220	rVB4	12127	18820	0.33%	0.027%
29	16.187	2240	2244	2248	rBV5	8951	12337	0.22%	0.018%
30	16.634	2317	2320	2323	rBV3	4409	7050	0.12%	0.010%
31	16.663	2323	2325	2329	rVB3	6281	6954	0.12%	0.010%
32	16.769	2336	2343	2350	rVB3	16778	27071	0.48%	0.039%
33	16.981	2373	2379	2389	rBV2	4018121	5698659	100.00%	8.263%
34	17.081	2390	2396	2410	rVB	3399133	4778652	83.86%	6.929%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
Data File : BN005255.D
Acq On : 24 Apr 2019 18:08
Operator : JU/SJ
Sample : PB119036BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK36

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	17.981	2545	2549	2553	rVB3	8962	11490	0.20%	0.017%
36	19.028	2723	2727	2730	rBV2	31605	41392	0.73%	0.060%
37	19.281	2766	2770	2775	rVB	25901	37398	0.66%	0.054%
38	19.392	2783	2789	2799	rBV	3473222	4828837	84.74%	7.002%
39	19.851	2865	2867	2870	rBV4	9658	13612	0.24%	0.020%
40	21.216	3094	3099	3110	rBV	3615358	4593145	80.60%	6.660%
41	21.851	3205	3207	3213	rVB4	67484	75392	1.32%	0.109%
42	22.310	3282	3285	3293	rVB4	137171	175252	3.08%	0.254%
43	22.810	3367	3370	3378	rVB	176299	256676	4.50%	0.372%
44	23.286	3444	3451	3459	rVV	2045128	3742676	65.68%	5.427%
45	23.374	3462	3466	3468	rVV	216551	325416	5.71%	0.472%
46	23.421	3468	3474	3487	rVB2	2290241	4352649	76.38%	6.311%
47	24.010	3569	3574	3580	rVB	181916	317777	5.58%	0.461%
48	24.739	3693	3698	3704	rVB2	176866	348392	6.11%	0.505%


Sum of corrected areas: 68966140

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042419\
Data File : BN005255.D
Acq On : 24 Apr 2019 18:08
Operator : JU/SJ
Sample : PB119036BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
SBLK36

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

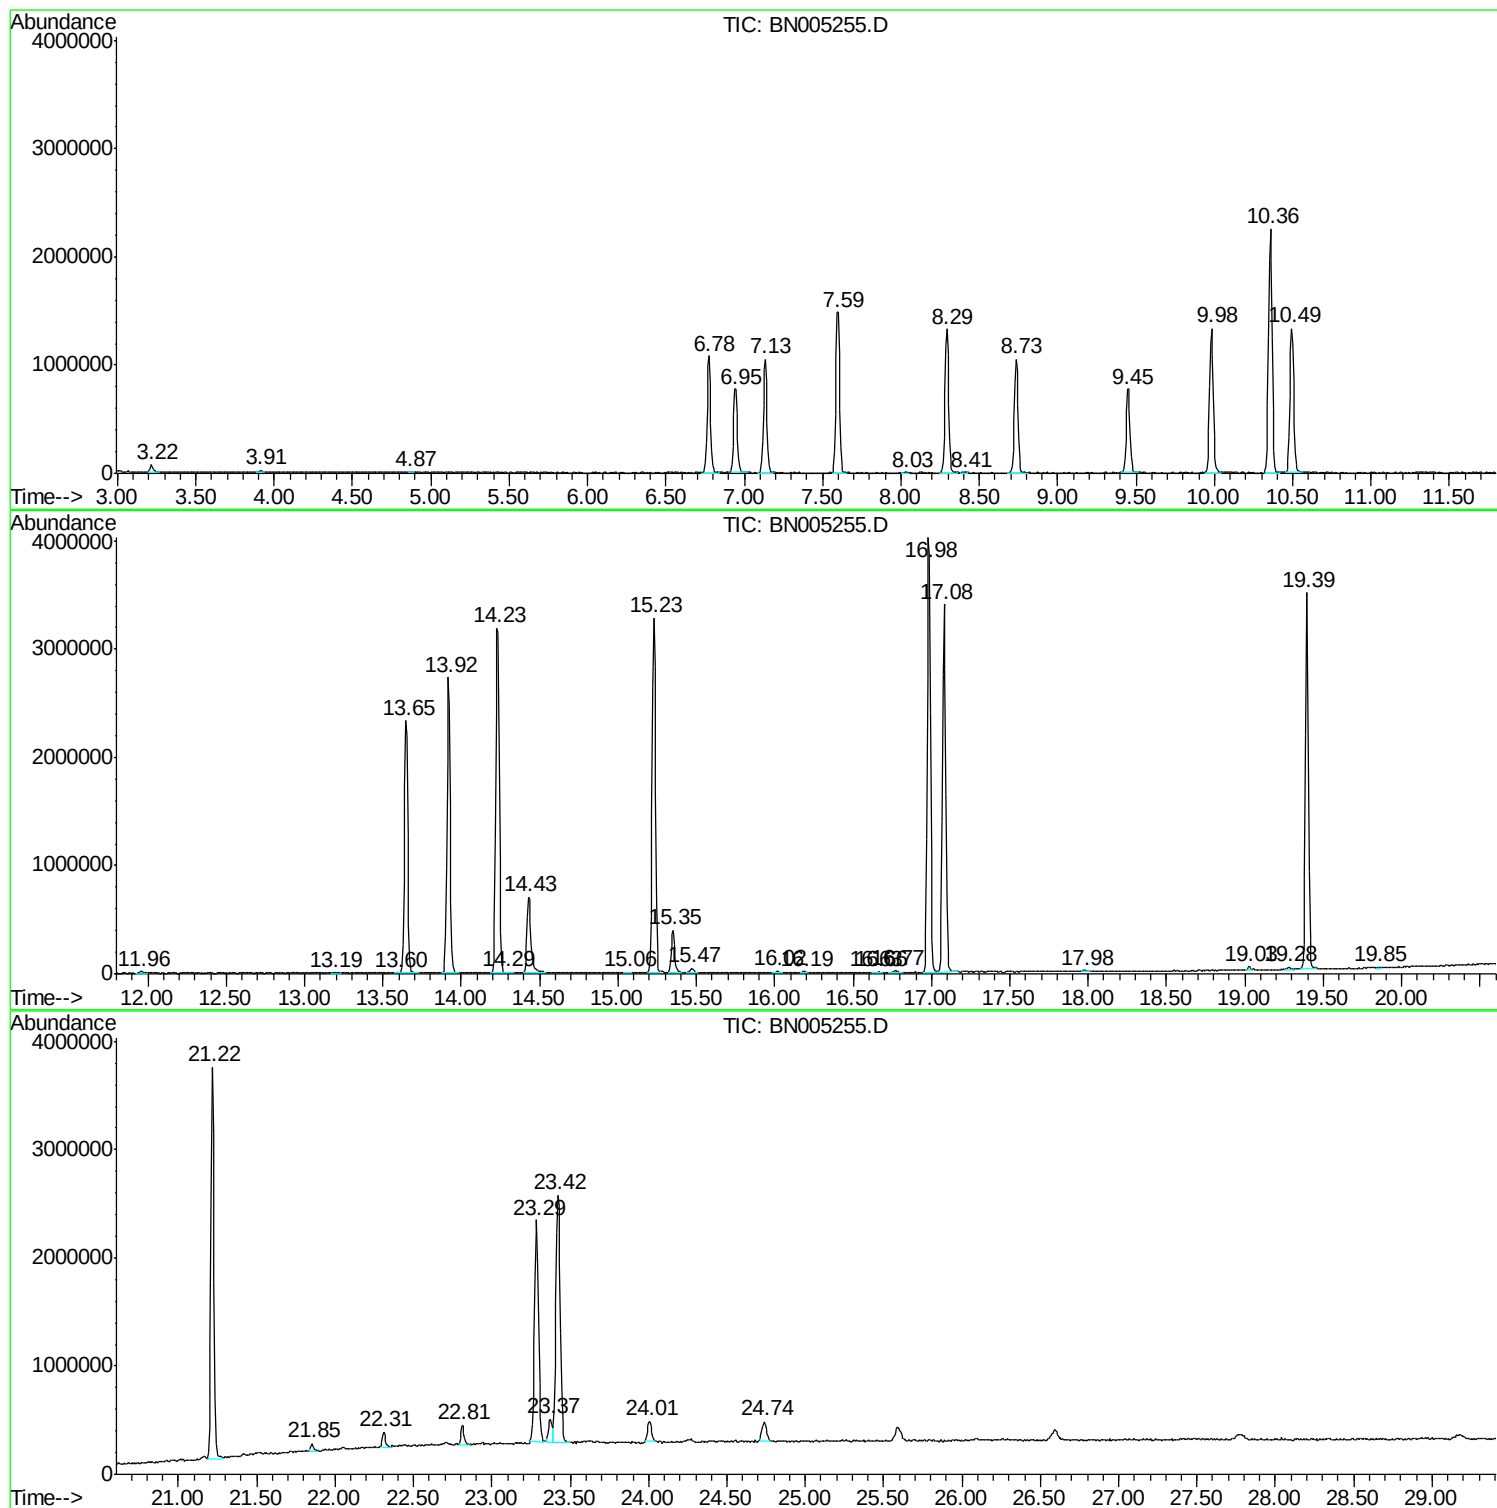

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
Data File : BN005255.D
Acq On : 24 Apr 2019 18:08
Operator : JU/SJ
Sample : PB119036BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK36

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042419\
Data File : BN005255.D
Acq On : 24 Apr 2019 18:08
Operator : JU/SJ
Sample : PB119036BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK36

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc