


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042420\
 Data File : BN010587.D
 Acq On : 24 Apr 2020 11:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 24 12:47:59 2020

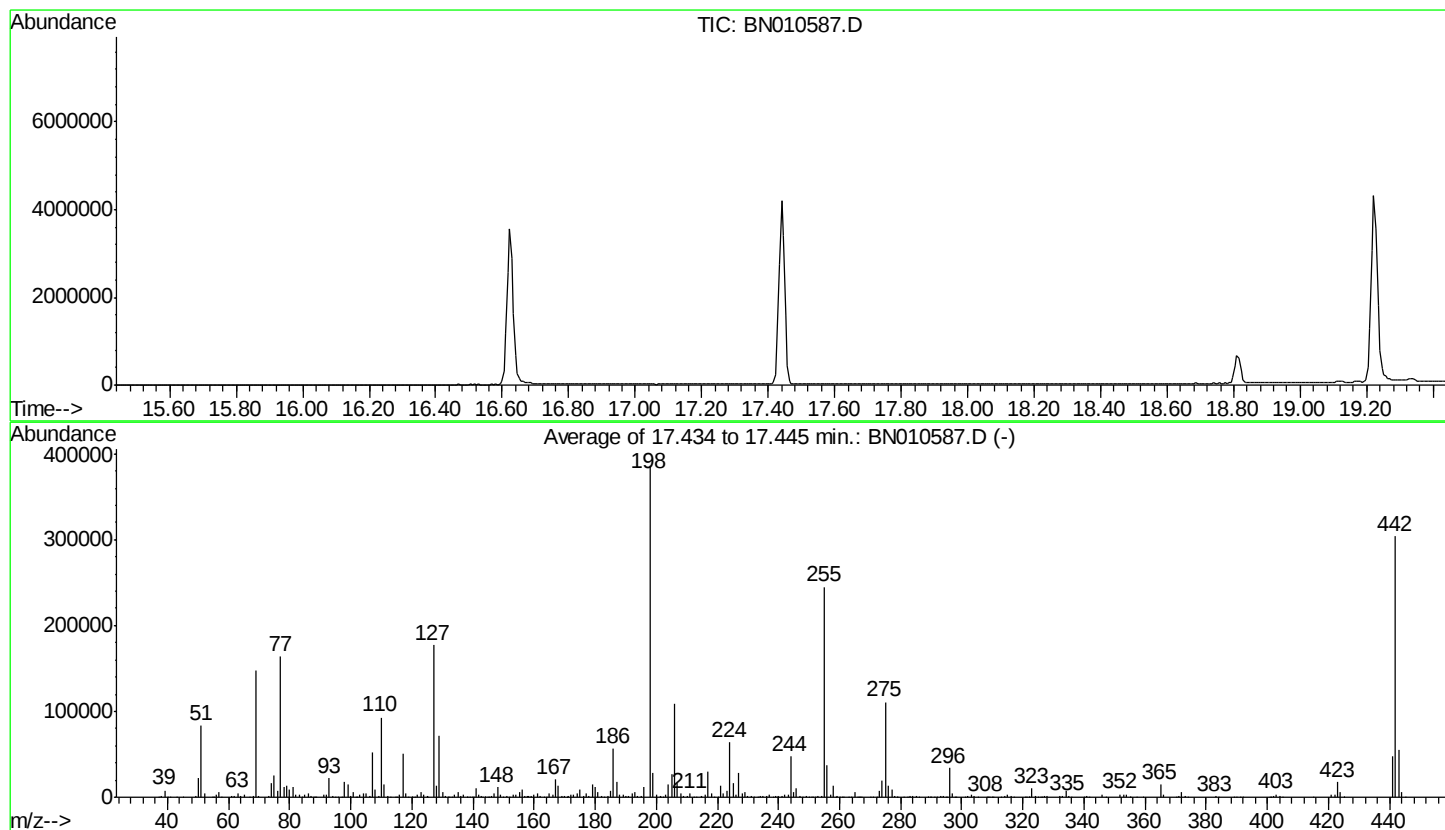

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	83050	PASS
68	69	0.00	2	0.6	953	PASS
69	198	0.00	100	38.2	147549	PASS
70	69	0.00	2	0.6	829	PASS
127	198	10	80	45.8	176810	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	386282	PASS
199	198	5	9	7.3	28170	PASS
275	198	10	60	28.7	110797	PASS
365	198	1	100	3.8	14799	PASS
441	198	0.01	100	12.3	47370	PASS
442	198	50	100	78.6	303594	PASS
443	442	15	24	18.4	55917	PASS