

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031201.D
 Acq On : 24 Apr 2024 23:29
 Operator : MA/JU
 Sample : P2104-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/26/2024
 Supervised By :mohammad ahmed 04/27/2024

Quant Time: Apr 25 00:44:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	151736	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.404	136	715357	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.275	164	494278	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.022	188	1115154	20.000	ng/u1	-0.01
79) Chrysene-d12	21.263	240	1210234	20.000	ng/u1	0.00
88) Perylene-d12	24.162	264	1361430	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	10452	3.218	ng/uL	0.00
4) Pyridine-d5	3.558	84	69501	7.431	ng/u1	0.00
7) Phenol-d5	6.805	99	217890	17.023	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	136644	18.349	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.163	132	183581	18.420	ng/u1	0.00
15) 4-Methylphenol-d8	8.334	113	123557	11.478	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	95633	18.606	ng/u1	0.00
24) 2-Nitrophenol-d4	9.498	143	97351	18.221	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.034	165	182648	17.336	ng/u1	0.00
31) 4-Chloroaniline-d4	10.551	131	240279	14.594	ng/u1	-0.01
46) Dimethylphthalate-d6	13.692	166	646770	18.804	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	742784	19.057	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.492	143	94706	13.192	ng/u1	0.00
60) Fluorene-d10	15.269	176	590011	19.705	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.398	200	59108	10.506	ng/u1	0.00
73) Anthracene-d10	17.122	188	936975	19.385	ng/u1	-0.01
81) Pyrene-d10	19.427	212	1282285	21.562	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.957	264	1377728	21.340	ng/u1	-0.02
Target Compounds					Qvalue	
16) Acetophenone	8.451	105	43029	2.580	ng/u1	98
72) Phenanthrene	17.069	178	175507	2.976	ng/u1	99
80) Fluoranthene	19.092	202	283883	4.033	ng/u1	99
82) Pyrene	19.457	202	246035	3.327	ng/u1	98
85) Benzo(a)anthracene	21.245	228	129054	1.570	ng/u1	98
87) Chrysene	21.304	228	128758	1.651	ng/u1	98
90) Benzo(b)fluoranthene	23.239	252	158080m	2.064	ng/u1	
93) Benzo(a)pyrene	24.021	252	106866	1.398	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031201.D
Acq On : 24 Apr 2024 23:29
Operator : MA/JU
Sample : P2104-10
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AB0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024


Quant Time: Apr 25 00:44:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

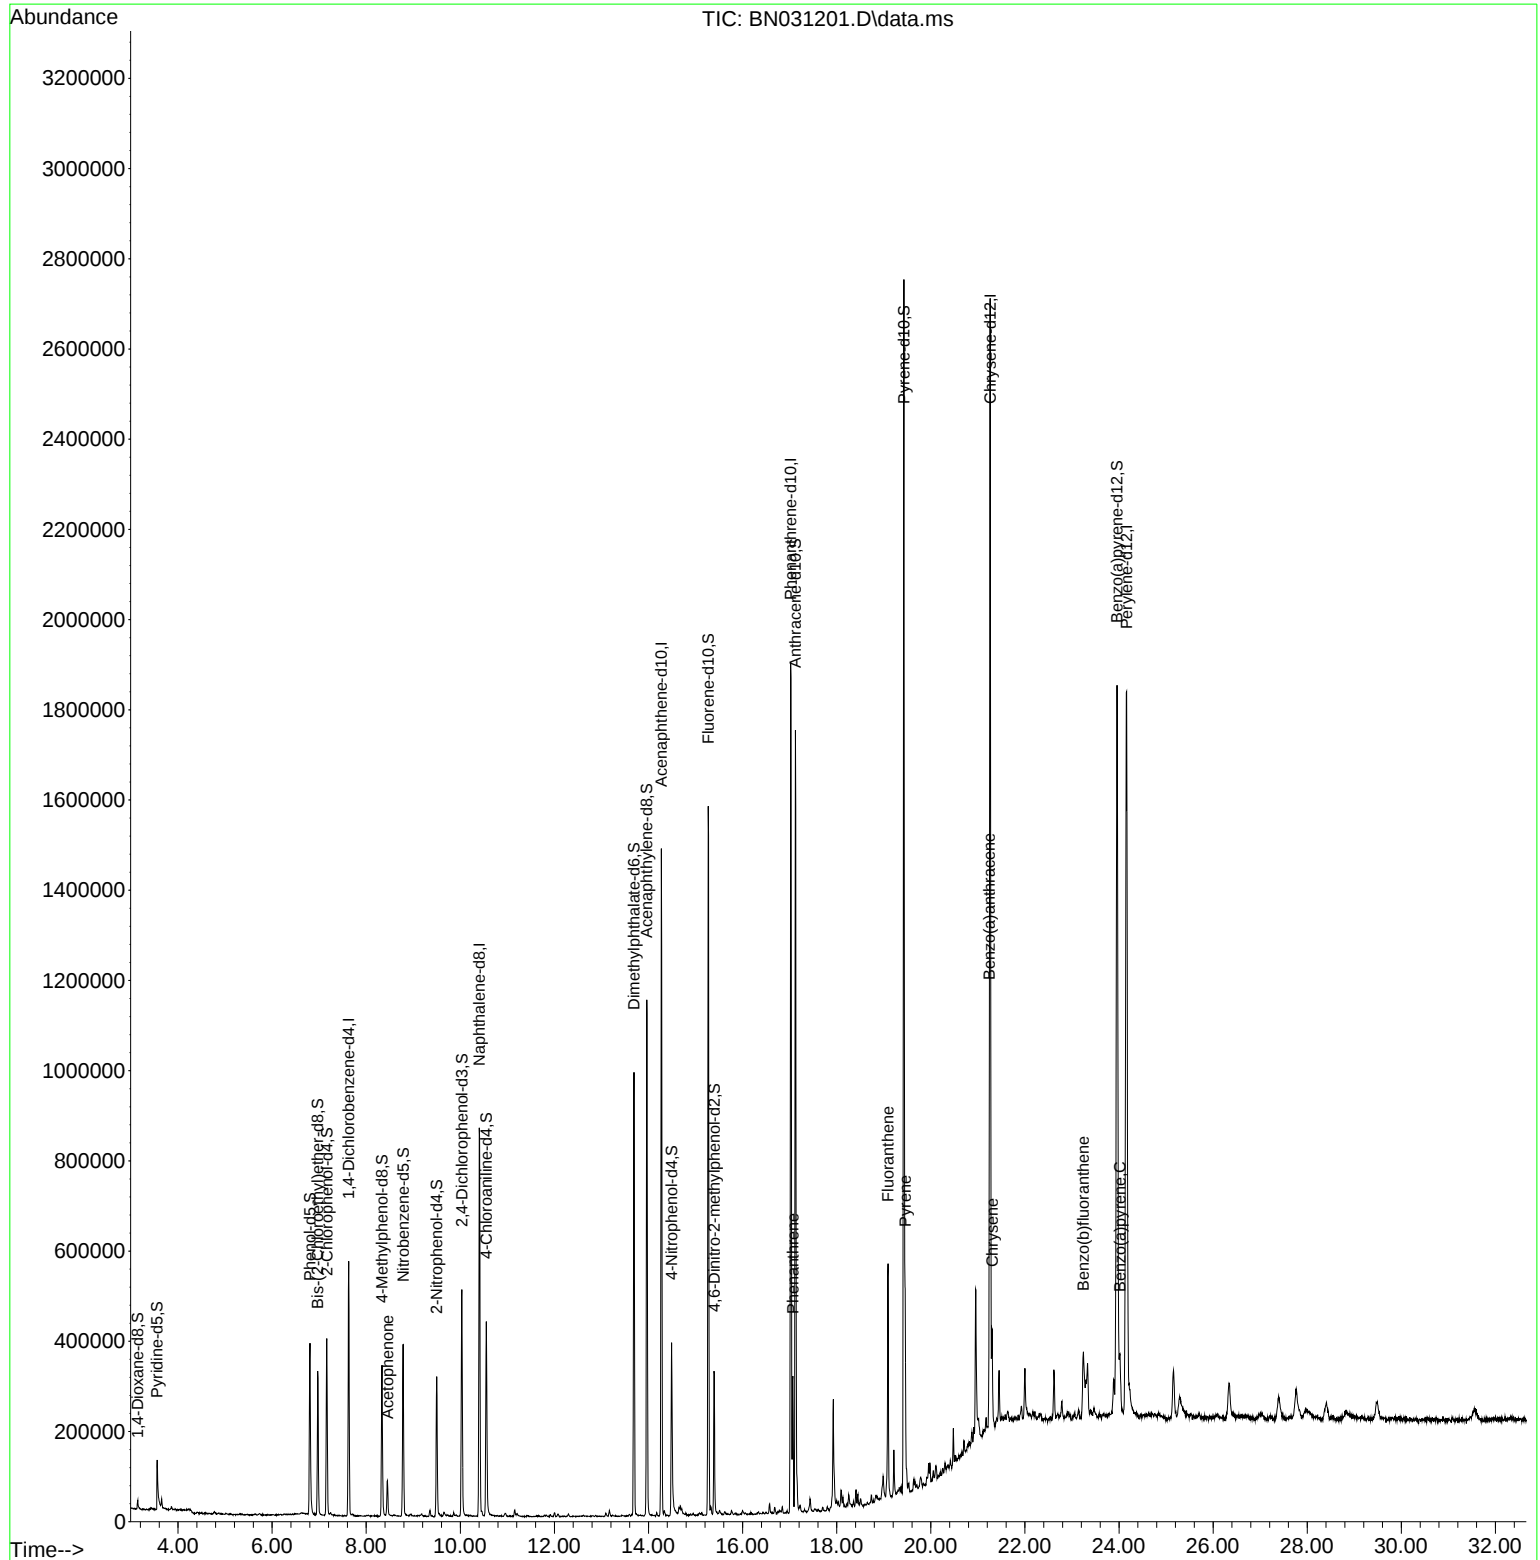

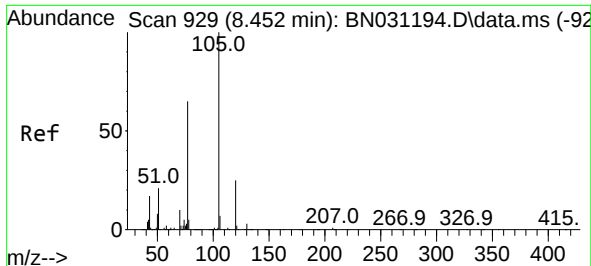

#16
Acetophenone
Concen: 2.580 ng/ul
RT: 8.451 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29




Instrument :
BNA_N
ClientSampleId :
C0AB0

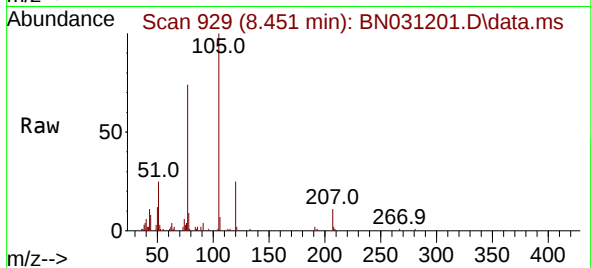


Tgt Ion:105 Resp: 43029
Ion Ratio Lower Upper
105 100
77 73.8 60.2 90.4
51 24.8 20.6 31.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

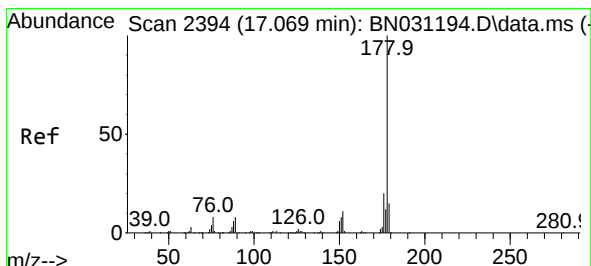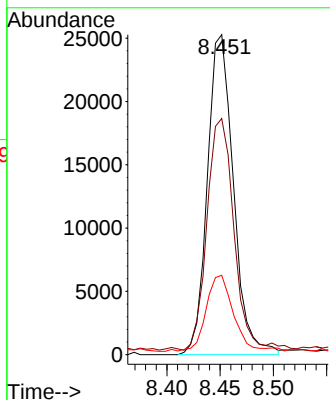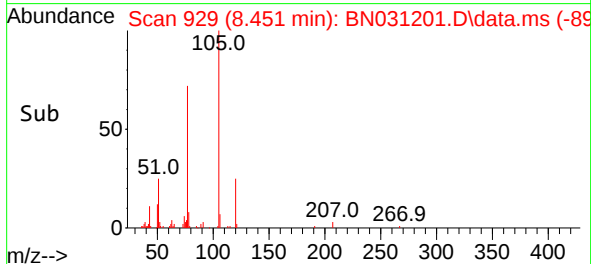


#72
Phenanthrene
Concen: 2.976 ng/ul
RT: 17.069 min Scan# 2394
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29

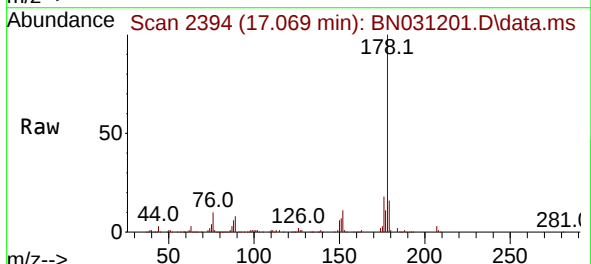


Tgt Ion:178 Resp: 175507
Ion Ratio Lower Upper
178 100
179 16.3 12.4 18.6
176 18.5 14.6 21.8

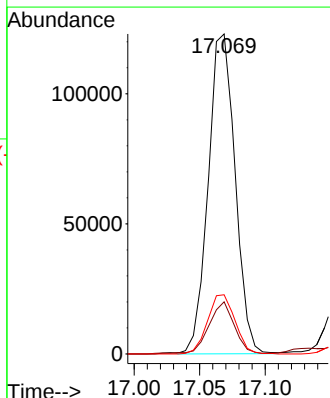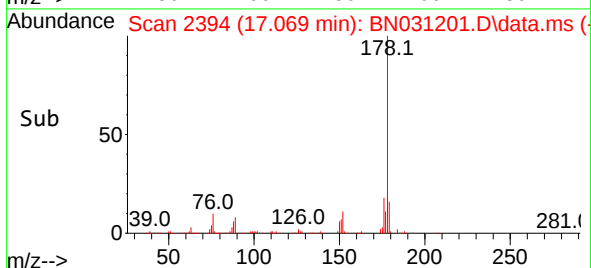

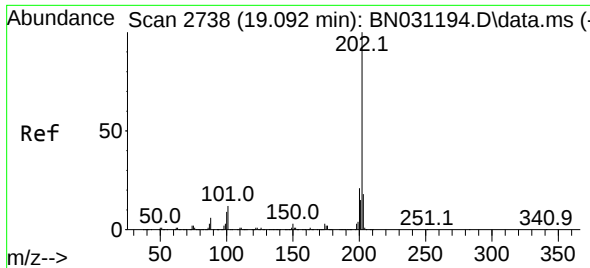

#80
Fluoranthene
Concen: 4.033 ng/u1
RT: 19.092 min Scan# 21
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29




Instrument :
BNA_N
ClientSampleId :
C0AB0

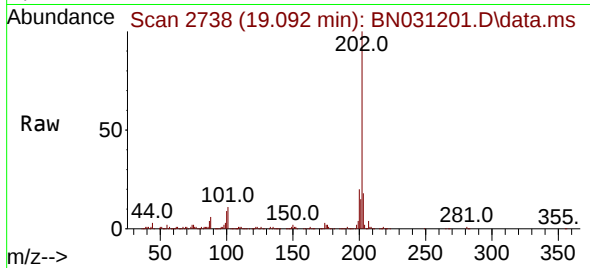


Tgt Ion:202 Resp: 28388
Ion Ratio Lower Upper
202 100
101 11.2 9.0 13.6
100 9.5 6.9 10.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

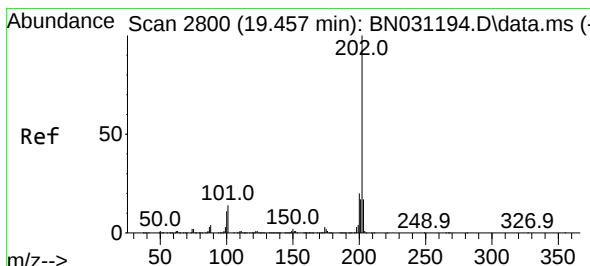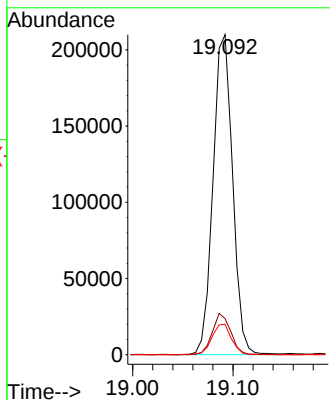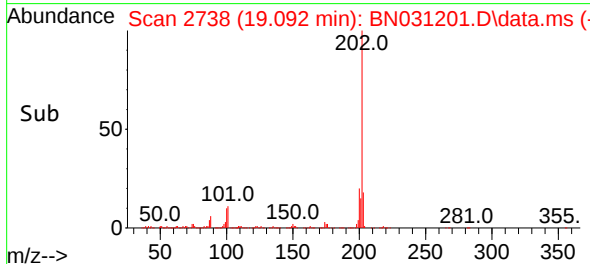


#82
Pyrene
Concen: 3.327 ng/u1
RT: 19.457 min Scan# 2800
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29

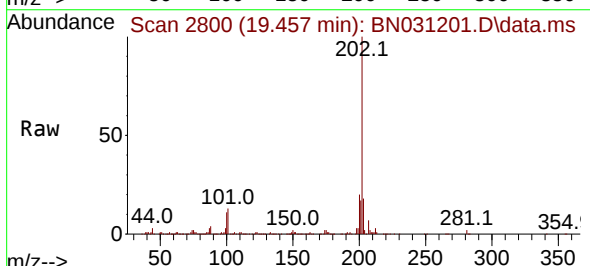


Tgt Ion:202 Resp: 246035
Ion Ratio Lower Upper
202 100
101 12.6 11.1 16.7
100 11.2 9.3 13.9

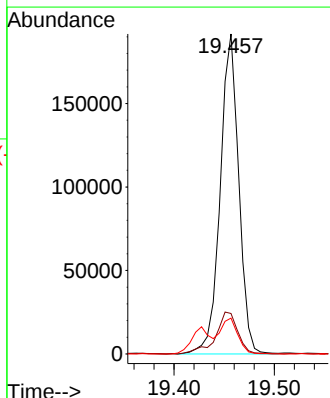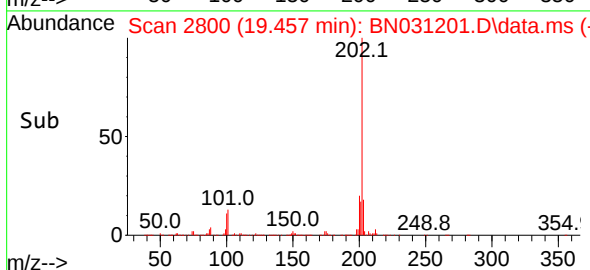

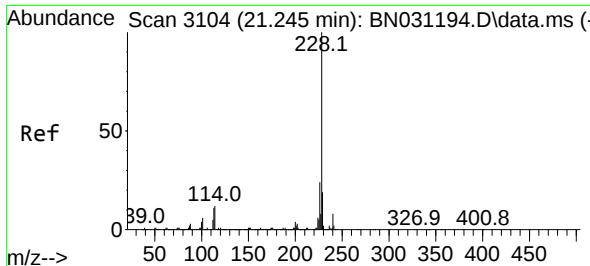

#85
Benzo(a)anthracene
Concen: 1.570 ng/u1
RT: 21.245 min Scan# 3104
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29




Instrument :
BNA_N
ClientSampleId :
C0AB0

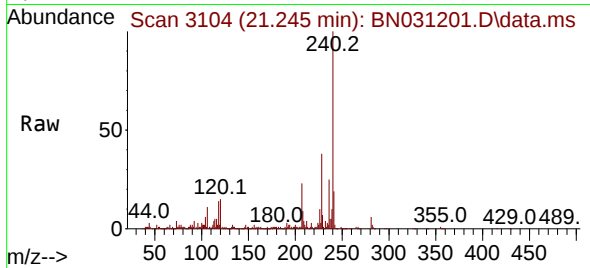

Tgt Ion:228 Resp: 129054
Ion Ratio Lower Upper
228 100
229 19.4 16.7 25.1
226 27.0 21.2 31.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 04/26/2024
Supervised By :mohammad ahmed 04/27/2024

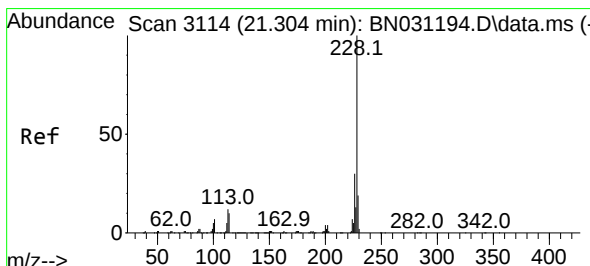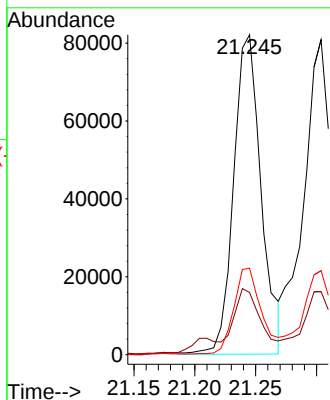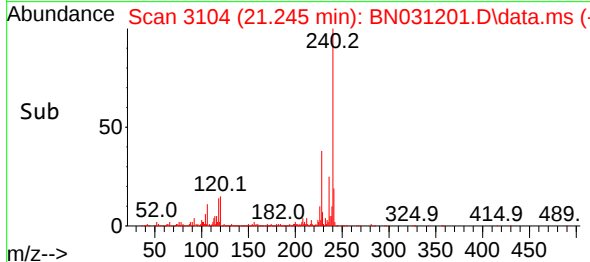

#87
Chrysene
Concen: 1.651 ng/u1
RT: 21.304 min Scan# 3114
Delta R.T. -0.006 min
Lab File: BN031201.D
Acq: 24 Apr 2024 23:29

Tgt Ion:228 Resp: 128758
Ion Ratio Lower Upper
228 100
226 26.7 22.6 34.0
229 20.0 15.8 23.8

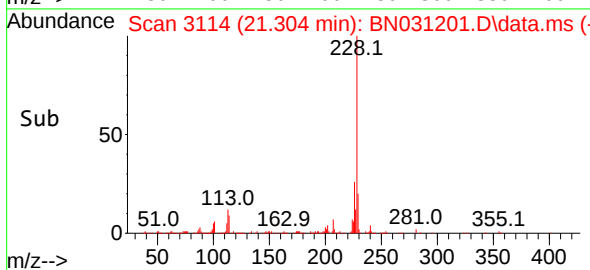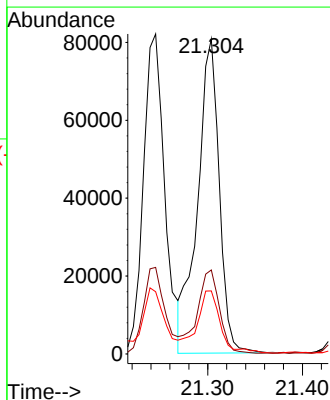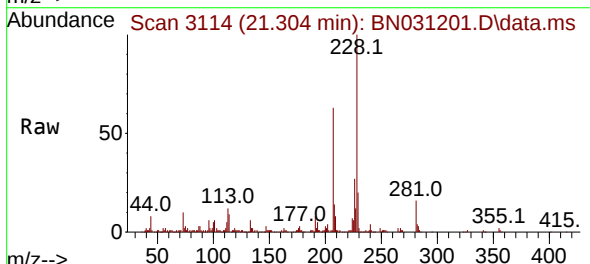

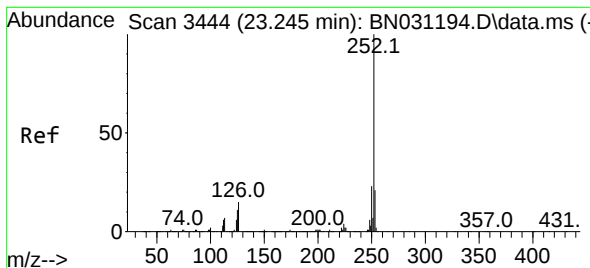

#90

Benzo(b)fluoranthene

Concen: 2.064 ng/ul m

RT: 23.239 min Scan# 3444

Delta R.T. -0.018 min

Lab File: BN031201.D


Acq: 24 Apr 2024 23:29

Instrument :

BNA_N

ClientSampleId :

C0AB0

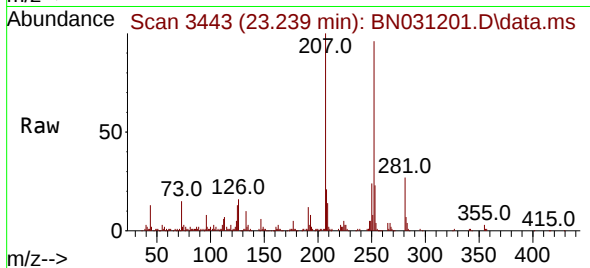

Tgt Ion:252 Resp: 158080

Ion Ratio Lower Upper

252 100

253 23.6 17.6 26.4




125 13.5 8.6 12.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/26/2024

Supervised By :mohammad ahmed 04/27/2024

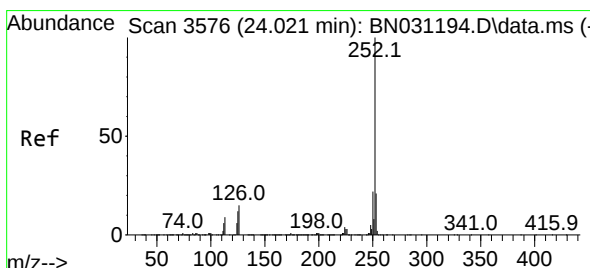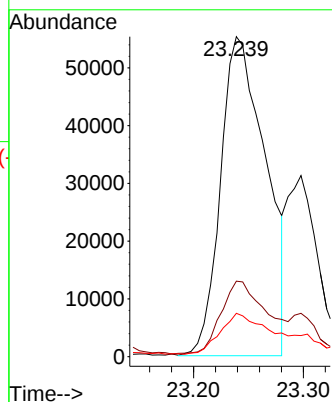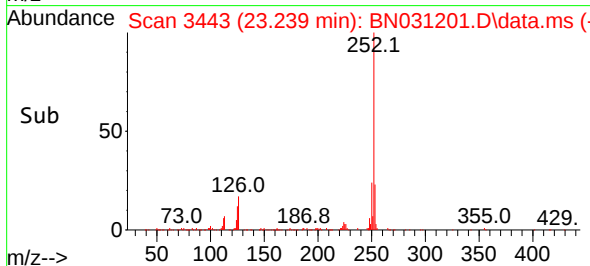

#93

Benzo(a)pyrene

Concen: 1.398 ng/ul

RT: 24.021 min Scan# 3576

Delta R.T. -0.012 min

Lab File: BN031201.D

Acq: 24 Apr 2024 23:29

Tgt Ion:252 Resp: 106866

Ion Ratio Lower Upper

252 100

253 21.5 17.7 26.5

125 13.4 9.9 14.9

