

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031202.D
 Acq On : 25 Apr 2024 00:09
 Operator : MA/JU
 Sample : P2104-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

Quant Time: Apr 25 00:42:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	213687	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.404	136	1008377	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.275	164	683371	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	1533438	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1681950	20.000	ng/ul	0.00
88) Perylene-d12	24.157	264	1834659	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	15675	3.427	ng/uL	0.00
4) Pyridine-d5	3.552	84	163801	12.435	ng/ul	0.00
7) Phenol-d5	6.805	99	363559	20.169	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	214337	20.437	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.163	132	293270	20.895	ng/ul	0.00
15) 4-Methylphenol-d8	8.334	113	250276	16.509	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	151277	20.880	ng/ul	0.00
24) 2-Nitrophenol-d4	9.498	143	158306	21.020	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	294909	19.857	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.551	131	407339	17.551	ng/ul	-0.01
46) Dimethylphthalate-d6	13.692	166	998629	21.000	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	1168502	21.684	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.492	143	180176	18.153	ng/ul	0.00
60) Fluorene-d10	15.275	176	907026	21.910	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	108241	13.991	ng/ul	0.00
73) Anthracene-d10	17.122	188	1473844	22.175	ng/ul	-0.01
81) Pyrene-d10	19.427	212	2020943	24.452	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	2161240	24.842	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.451	105	55676	2.370	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031202.D
Acq On : 25 Apr 2024 00:09
Operator : MA/JU
Sample : P2104-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC6


Quant Time: Apr 25 00:42:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

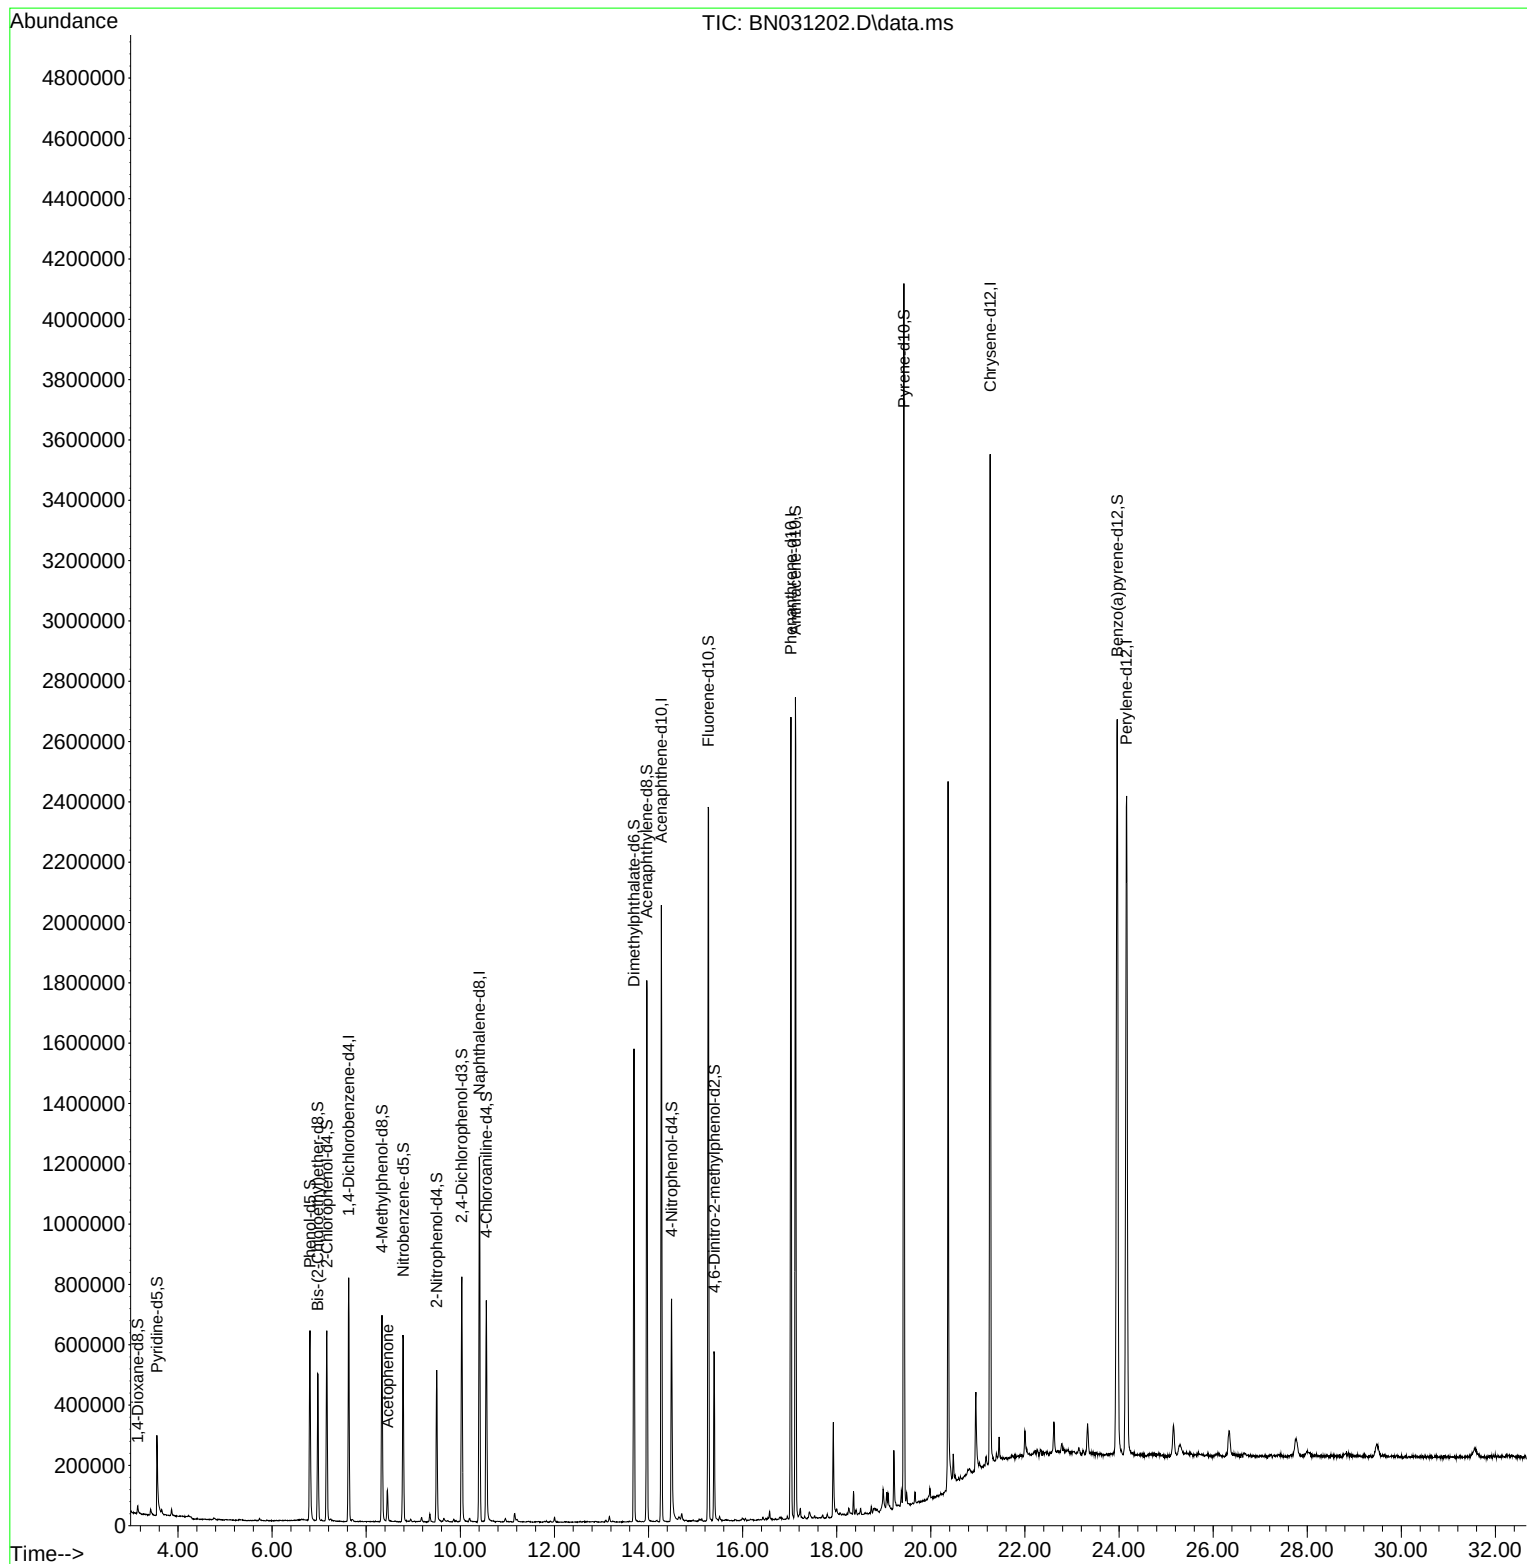

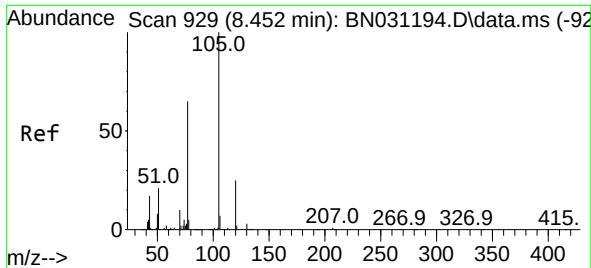

#16
 Acetophenone
 Concen: 2.370 ng/ul
 RT: 8.451 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN031202.D
 Acq: 25 Apr 2024 00:09

Instrument :
 BNA_N
 ClientSampleId :
 C0AC6

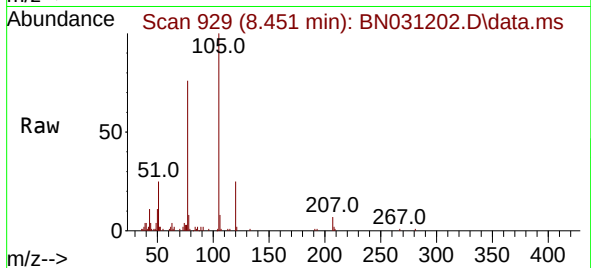

Tgt Ion:	105	Resp:	55676
Ion	Ratio	Lower	Upper
105	100		
77	76.4	60.2	90.4
51	25.2	20.6	31.0

