

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031205.D
 Acq On : 25 Apr 2024 02:08
 Operator : MA/JU
 Sample : P2104-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AL7

Quant Time: Apr 25 02:38:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	177268	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.404	136	821434	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.275	164	554602	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	1158341	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1319146	20.000	ng/u1	0.00
88) Perylene-d12	24.157	264	1593035	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	11293	2.976	ng/uL	0.00
4) Pyridine-d5	3.558	84	65388	5.984	ng/u1	0.00
7) Phenol-d5	6.805	99	254150	16.996	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	156640	18.004	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.163	132	213474	18.335	ng/u1	0.00
15) 4-Methylphenol-d8	8.334	113	169088	13.445	ng/u1	0.00
21) Nitrobenzene-d5	8.781	128	110304	18.689	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.499	143	110365	17.990	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.034	165	212491	17.564	ng/u1	0.00
31) 4-Chloroaniline-d4	10.552	131	293924	15.547	ng/u1	-0.01
46) Dimethylphthalate-d6	13.693	166	709230	18.377	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	862763	19.728	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.493	143	103785	12.884	ng/u1	0.00
60) Fluorene-d10	15.269	176	664981	19.793	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.398	200	60807	10.405	ng/u1	0.00
73) Anthracene-d10	17.122	188	1034373	20.602	ng/u1	-0.01
81) Pyrene-d10	19.428	212	1334211	20.583	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.963	264	1502581	19.890	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.446	105	47535	2.440	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031205.D
Acq On : 25 Apr 2024 02:08
Operator : MA/JU
Sample : P2104-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COAL7


Quant Time: Apr 25 02:38:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

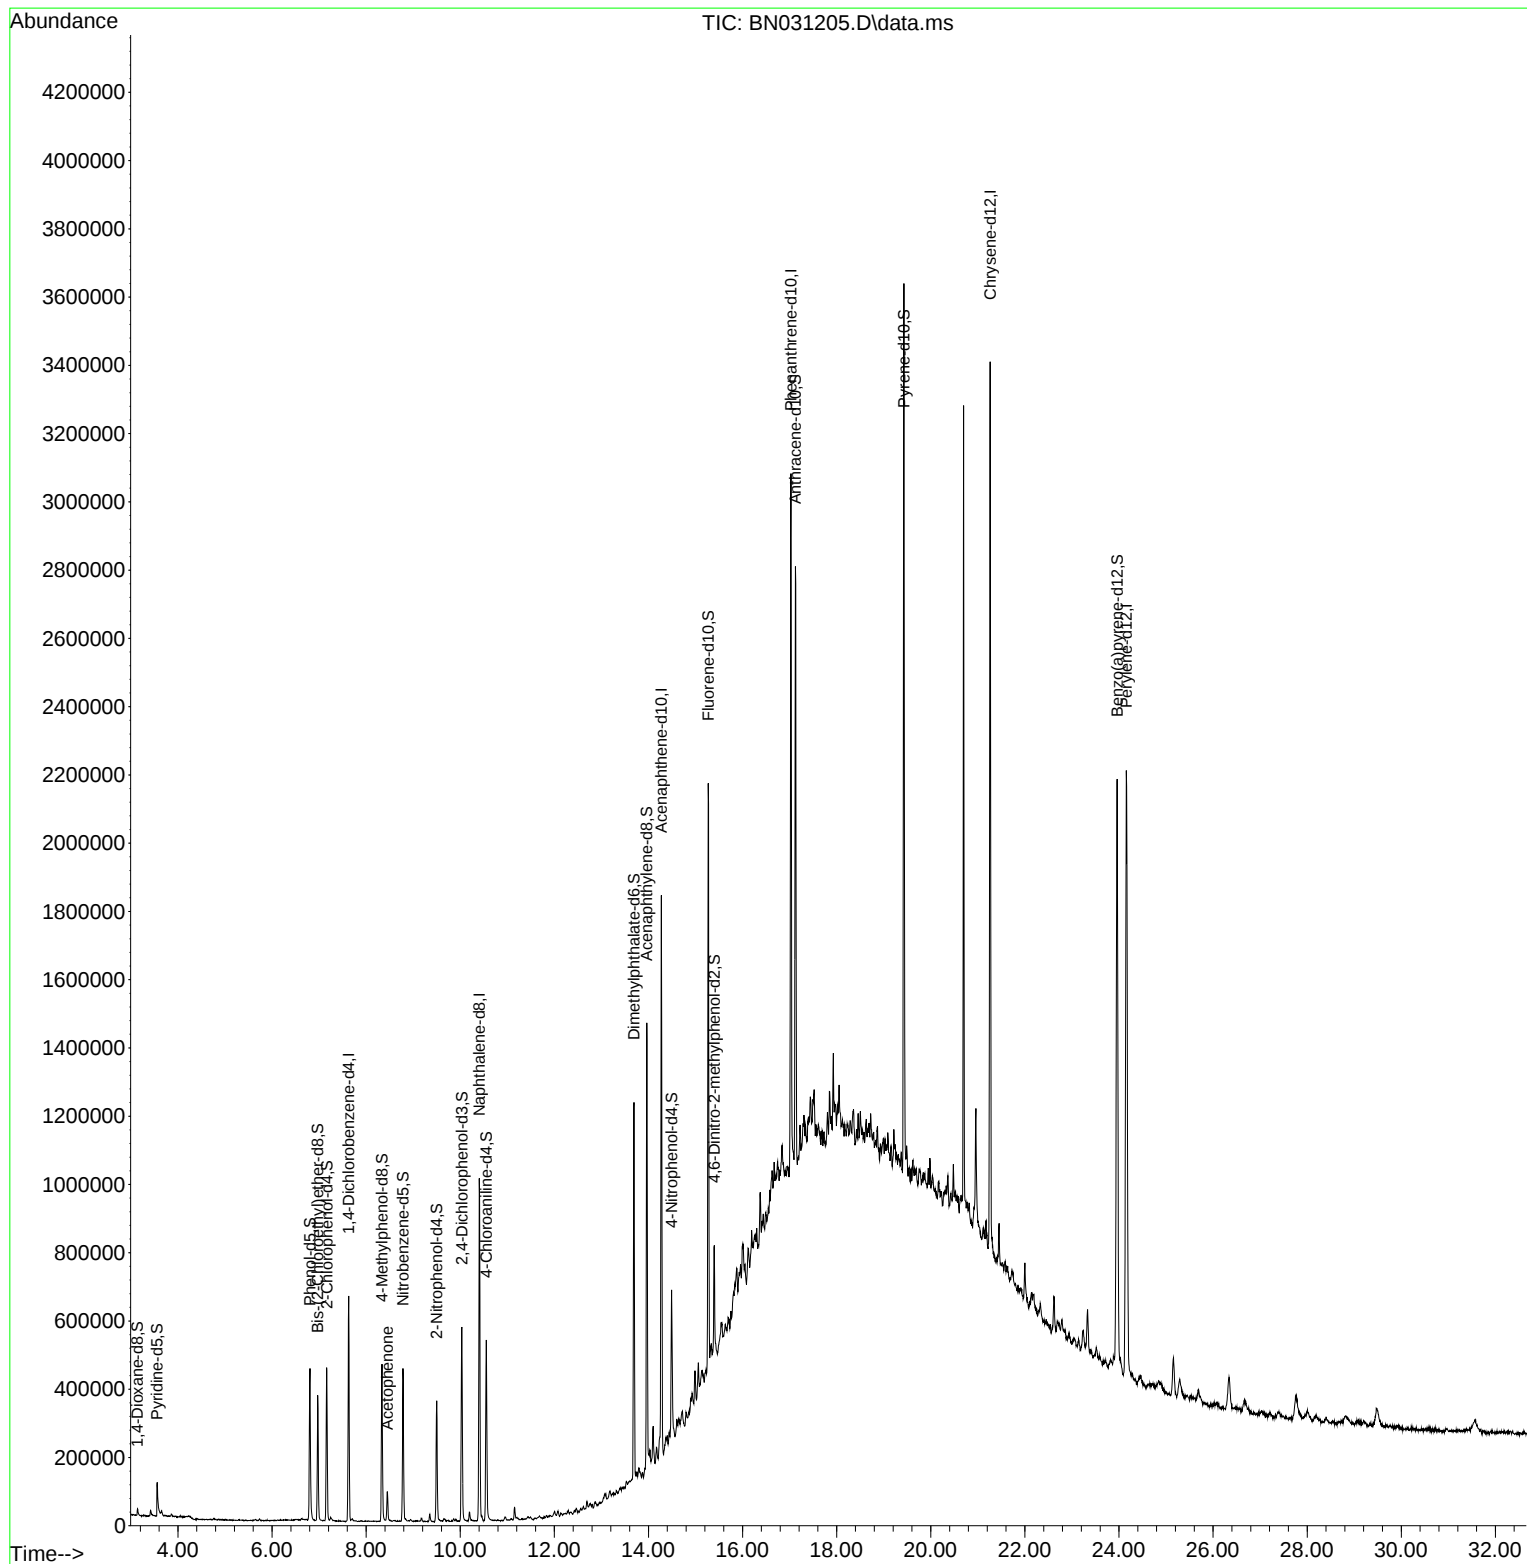

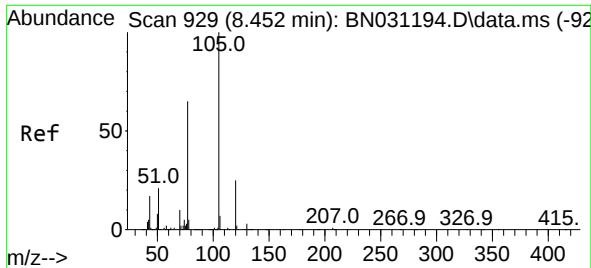

#16
 Acetophenone
 Concen: 2.440 ng/ul
 RT: 8.446 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BN031205.D
 Acq: 25 Apr 2024 02:08

Instrument :
 BNA_N
 ClientSampleId :
 C0AL7

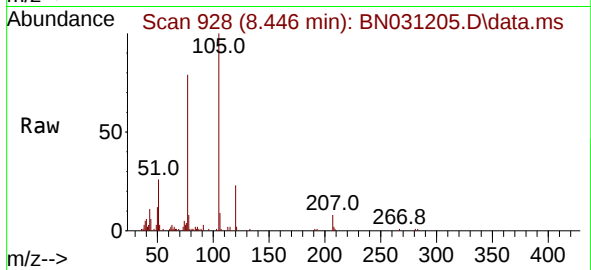

Tgt Ion:	105	Resp:	47535
Ion	Ratio	Lower	Upper
105	100		
77	79.3	60.2	90.4
51	26.3	20.6	31.0

