

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031210.D
 Acq On : 25 Apr 2024 06:07
 Operator : MA/JU
 Sample : P2104-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA0

Quant Time: Apr 25 06:39:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	215776	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.405	136	994068	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.275	164	672026	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	1512035	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1563653	20.000	ng/u1	0.00
88) Perylene-d12	24.163	264	1627799	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.146	96	17741	3.841	ng/uL	0.00
4) Pyridine-d5	3.558	84	70784	5.322	ng/u1	0.00
7) Phenol-d5	6.805	99	381232	20.944	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	249005	23.513	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.158	132	337183	23.791	ng/u1	-0.01
15) 4-Methylphenol-d8	8.334	113	218992	14.306	ng/u1	0.00
21) Nitrobenzene-d5	8.781	128	179973	25.198	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.499	143	185863	25.035	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.028	165	329297	22.492	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.552	131	408901	17.872	ng/u1	-0.01
46) Dimethylphthalate-d6	13.693	166	1130783	24.180	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	1315520	24.824	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.493	143	151748	15.547	ng/u1	0.00
60) Fluorene-d10	15.269	176	1023761	25.148	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.398	200	120368	15.779	ng/u1	0.00
73) Anthracene-d10	17.122	188	1627527	24.834	ng/u1	-0.01
81) Pyrene-d10	19.428	212	2143230	27.893	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.963	264	2002434	25.941	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.452	105	69293	2.922	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031210.D
Acq On : 25 Apr 2024 06:07
Operator : MA/JU
Sample : P2104-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA0

Quant Time: Apr 25 06:39:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

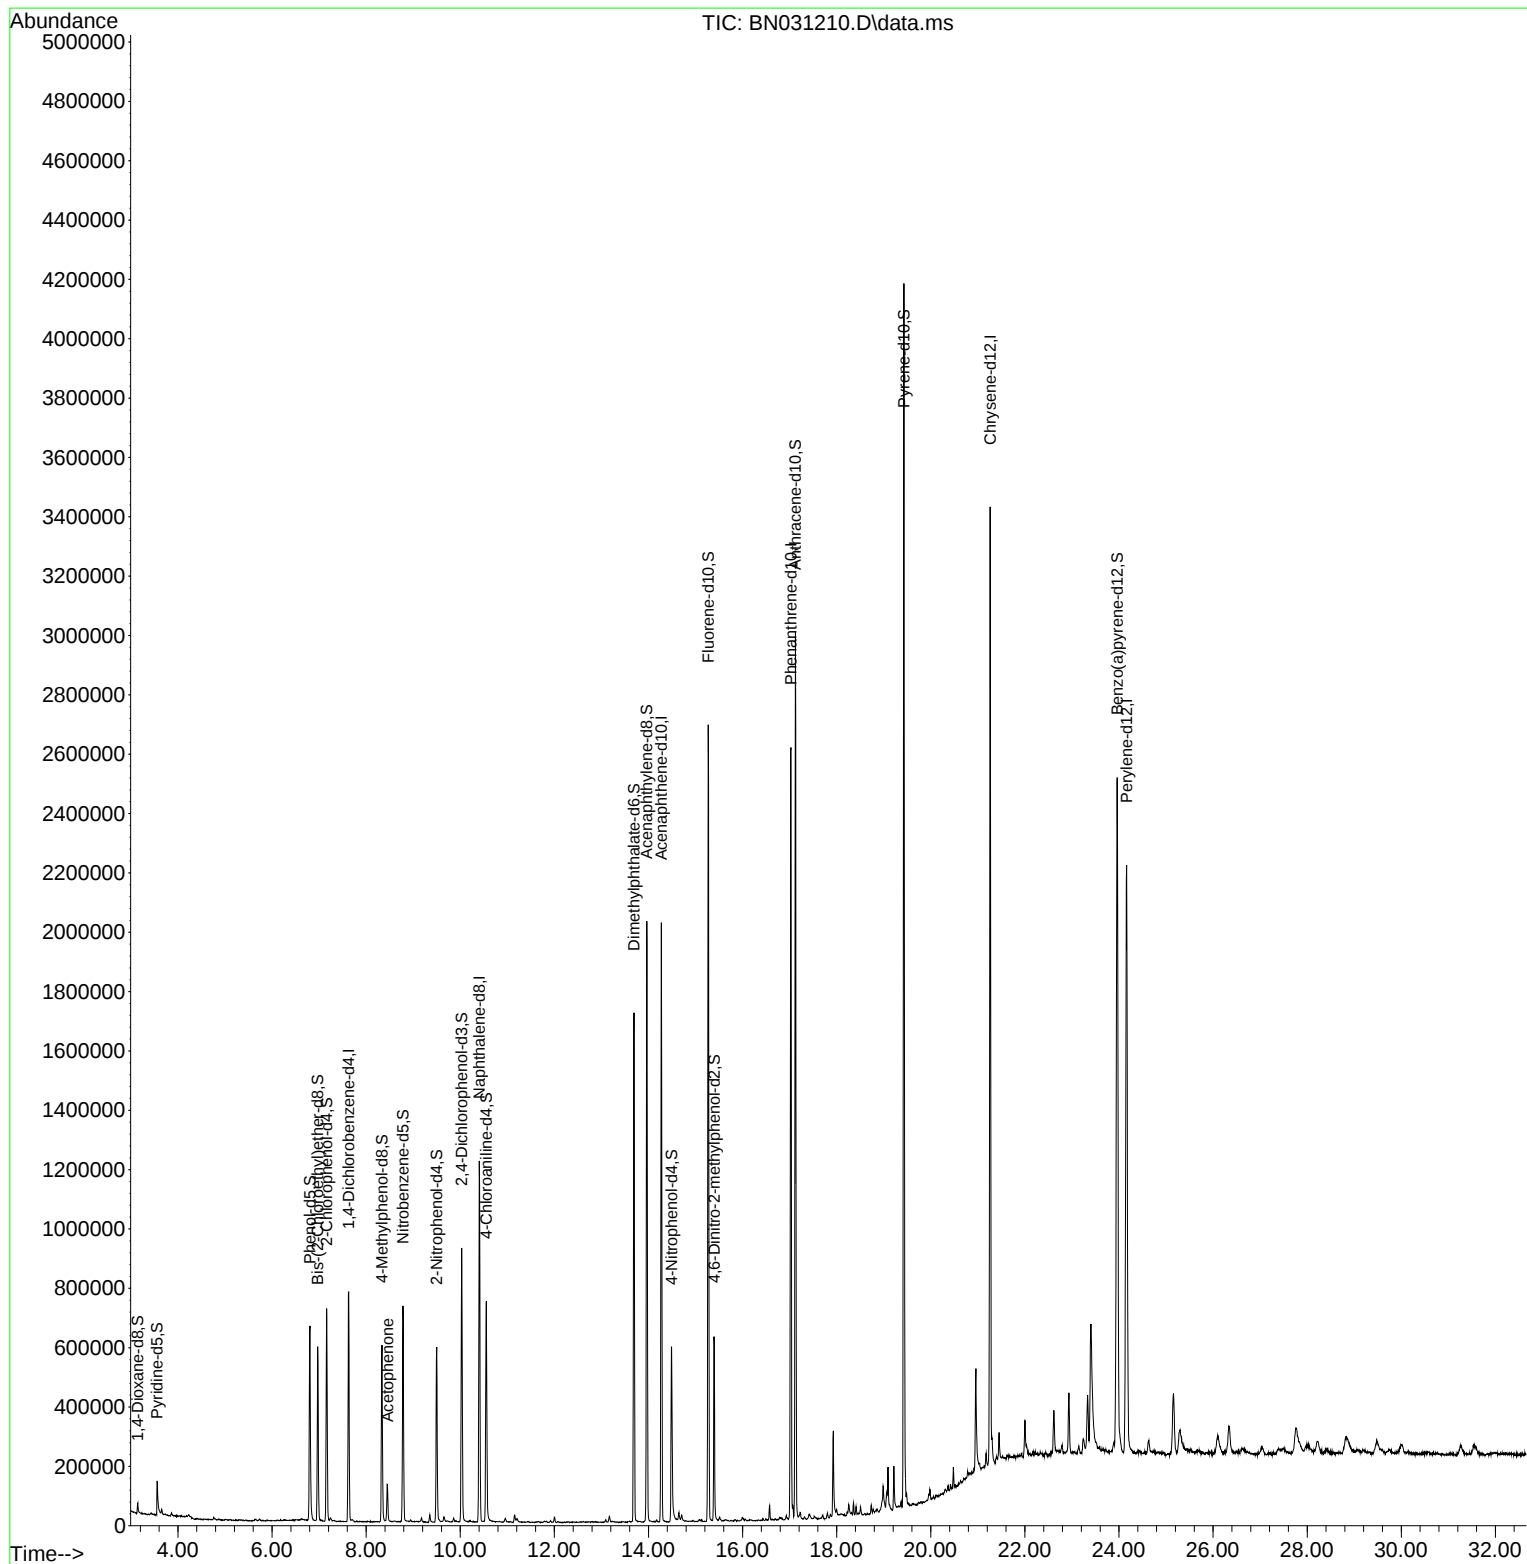

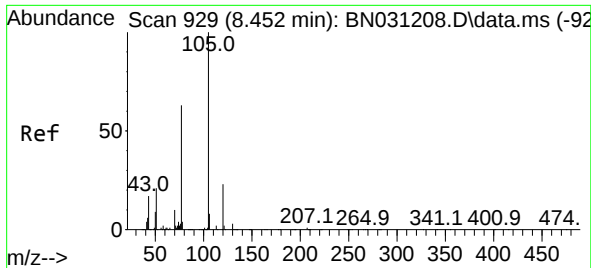

#16
 Acetophenone
 Concen: 2.922 ng/ul
 RT: 8.452 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BN031210.D
 Acq: 25 Apr 2024 06:07

Instrument :
 BNA_N
 ClientSampleId :
 C0AA0

Tgt Ion:105 Resp: 69293
 Ion Ratio Lower Upper
 105 100
 77 75.8 60.2 90.4
 51 26.1 20.6 31.0

