

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031195.D
 Acq On : 24 Apr 2024 19:30
 Operator : MA/JU
 Sample : PB160461BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK461

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	41	rVB	34584	53981	1.08%	0.107%
2	3.546	92	95	116	rBV	461311	826432	16.57%	1.637%
3	3.864	145	149	154	rVB	10253	14052	0.28%	0.028%
4	6.805	642	649	665	rVB	681163	1062026	21.30%	2.104%
5	6.969	669	677	686	rBV	525916	835987	16.77%	1.656%
6	7.164	703	710	720	rBV	681143	1072868	21.52%	2.126%
7	7.628	782	789	799	rBV	657355	1022604	20.51%	2.026%
8	8.334	902	909	924	rBV	870790	1388628	27.85%	2.751%
9	8.787	977	986	999	rBV	667410	1081697	21.69%	2.143%
10	9.499	1098	1107	1119	rBV	547070	880348	17.65%	1.744%
11	10.034	1190	1198	1212	rBV	857610	1458389	29.25%	2.890%
12	10.405	1254	1261	1275	rBV	999415	1690527	33.90%	3.350%
13	10.552	1279	1286	1302	rBV	916872	1554898	31.18%	3.081%
14	12.005	1527	1533	1540	rBV	14753	25993	0.52%	0.052%
15	13.169	1725	1731	1736	rBV2	16248	26549	0.53%	0.053%
16	13.693	1813	1820	1831	rBV	1639068	2233440	44.79%	4.425%
17	13.969	1860	1867	1878	rBV	1815970	2745956	55.07%	5.441%
18	14.275	1912	1919	1931	rBV	1690808	2423592	48.60%	4.802%
19	14.493	1949	1956	1978	rBV	639318	1149850	23.06%	2.278%
20	15.275	2082	2089	2101	rBV	2418877	3479125	69.77%	6.893%
21	15.398	2104	2110	2120	rBV	585872	829222	16.63%	1.643%
22	15.516	2125	2130	2136	rVB4	12606	21517	0.43%	0.043%
23	16.057	2219	2222	2228	rVB6	5806	8366	0.17%	0.017%
24	17.028	2381	2387	2397	rBV	2219693	3086921	61.91%	6.116%
25	17.122	2397	2403	2419	rVB2	2793089	4008218	80.38%	7.942%
26	18.992	2716	2721	2726	rBV2	33642	50161	1.01%	0.099%
27	19.057	2729	2732	2739	rVB	32807	47563	0.95%	0.094%
28	19.369	2782	2785	2788	rVB2	9143	11347	0.23%	0.022%
29	19.428	2789	2795	2805	rBV2	3689347	4986421	100.00%	9.880%
30	21.263	3101	3107	3116	rBV	2627762	3728005	74.76%	7.386%
31	23.963	3557	3566	3580	rVB2	2082551	4949362	99.26%	9.806%
32	24.157	3591	3599	3612	rVB	1561930	3716834	74.54%	7.364%




Sum of corrected areas: 50470879

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031195.D
Acq On : 24 Apr 2024 19:30
Operator : MA/JU
Sample : PB160461BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

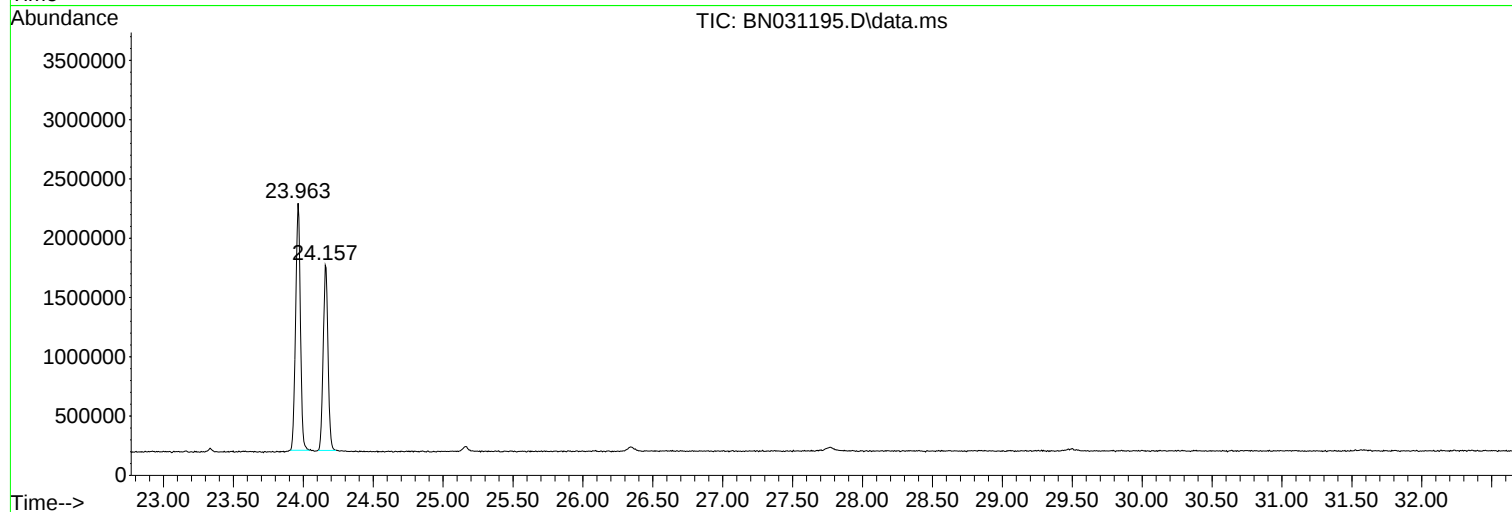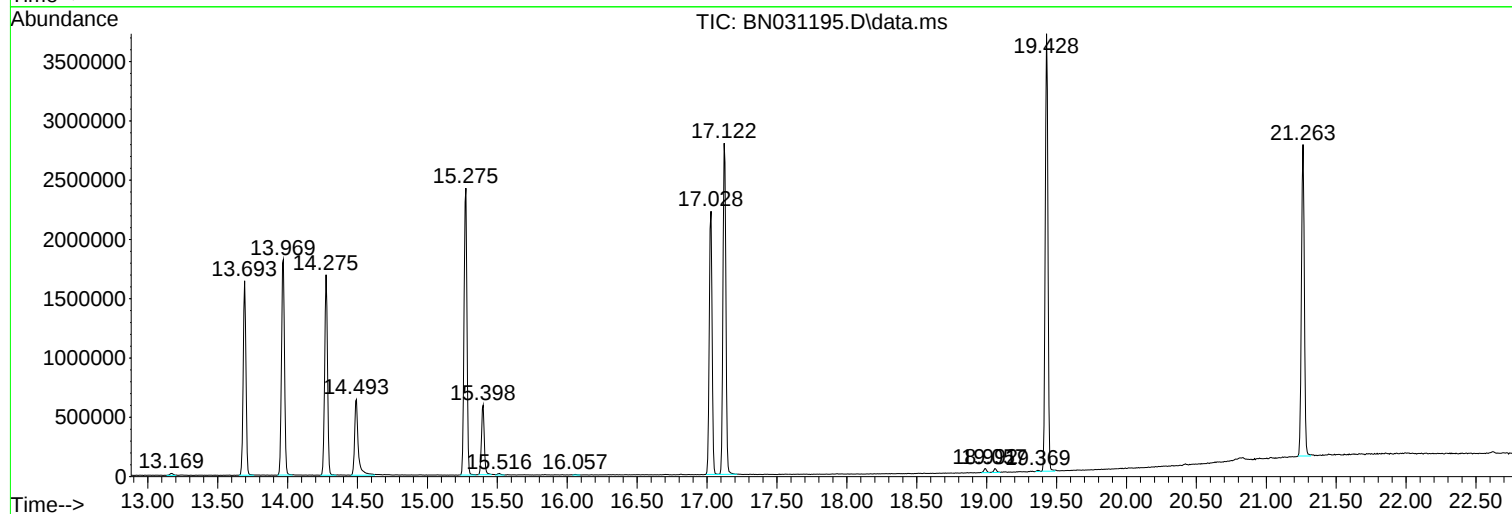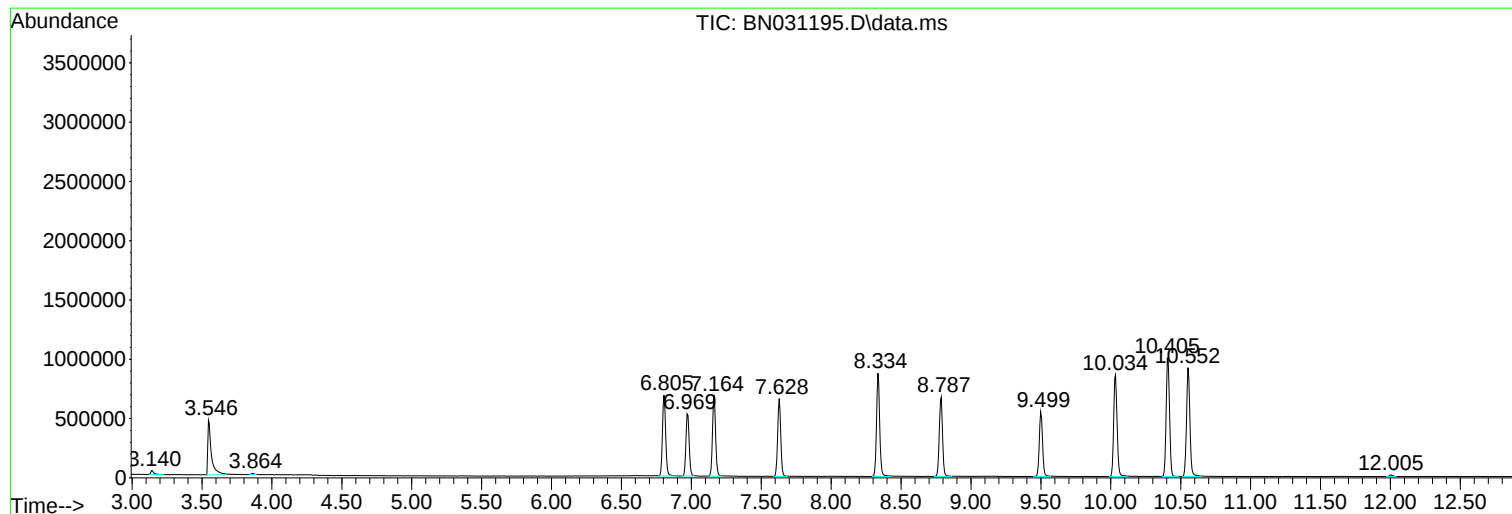

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031195.D
Acq On : 24 Apr 2024 19:30
Operator : MA/JU
Sample : PB160461BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031195.D
Acq On : 24 Apr 2024 19:30
Operator : MA/JU
Sample : PB160461BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK461

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc