

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
 Data File : BN031209.D
 Acq On : 25 Apr 2024 05:27
 Operator : MA/JU
 Sample : PB160442BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK442

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031209.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	23	26	41	rVB	37343	67503	1.18%	0.121%
2	3.546	92	95	120	rBV	477243	867323	15.16%	1.557%
3	3.864	145	149	158	rVB2	11725	19141	0.33%	0.034%
4	5.346	398	401	406	rBV7	2970	6167	0.11%	0.011%
5	6.805	642	649	663	rVB	708931	1133706	19.82%	2.035%
6	6.969	671	677	687	rVB	577498	887229	15.51%	1.593%
7	7.158	702	709	718	rBV	715235	1161082	20.30%	2.085%
8	7.628	782	789	798	rBV	699024	1106380	19.34%	1.986%
9	8.334	902	909	922	rBV	928579	1489697	26.04%	2.674%
10	8.781	978	985	996	rBV	720943	1170068	20.45%	2.101%
11	9.499	1098	1107	1117	rBV	589329	974989	17.04%	1.750%
12	10.028	1190	1197	1213	rBV	928287	1584664	27.70%	2.845%
13	10.404	1253	1261	1271	rBV	1104313	1833820	32.05%	3.292%
14	10.551	1276	1286	1304	rBV	981652	1673278	29.25%	3.004%
15	11.998	1528	1532	1538	rVB	15270	22748	0.40%	0.041%
16	13.169	1724	1731	1737	rVB	19544	32387	0.57%	0.058%
17	13.234	1737	1742	1744	rBV5	4634	6720	0.12%	0.012%
18	13.692	1812	1820	1831	rBV	1658650	2393320	41.83%	4.297%
19	13.963	1860	1866	1878	rBV	1960329	2952269	51.60%	5.300%
20	14.275	1911	1919	1929	rBV	1847237	2678491	46.82%	4.809%
21	14.487	1949	1955	1976	rBV	726314	1285846	22.48%	2.309%
22	15.269	2082	2088	2096	rBV	2584496	3691820	64.53%	6.628%
23	15.398	2103	2110	2125	rBV	685802	1000484	17.49%	1.796%
24	15.510	2125	2129	2135	rVB6	13263	20933	0.37%	0.038%
25	16.063	2218	2223	2228	rVB8	6481	11181	0.20%	0.020%
26	16.810	2347	2350	2356	rVB3	4510	5914	0.10%	0.011%
27	17.028	2380	2387	2397	rBV	2340352	3469184	60.64%	6.228%
28	17.122	2397	2403	2417	rVV2	2977869	4284018	74.88%	7.691%
29	17.928	2536	2540	2542	rBV4	4504	6407	0.11%	0.012%
30	18.992	2716	2721	2725	rBV	40262	52209	0.91%	0.094%
31	19.063	2728	2733	2738	rBV	36792	54035	0.94%	0.097%
32	19.369	2781	2785	2788	rVB4	19876	23900	0.42%	0.043%
33	19.427	2789	2795	2802	rBV	3948998	5283186	92.35%	9.485%
34	20.416	2961	2963	2967	rBV5	20622	22491	0.39%	0.040%
35	21.263	3101	3107	3114	rBV	2908636	4211674	73.62%	7.561%
36	23.962	3557	3566	3581	rVB2	2321907	5720900	100.00%	10.271%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031209.D
Acq On : 25 Apr 2024 05:27
Operator : MA/JU
Sample : PB160442BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK442

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	24.162	3591	3600	3613	rVB	1826120	4495302	78.58%	8.070%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 55700466

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031209.D
Acq On : 25 Apr 2024 05:27
Operator : MA/JU
Sample : PB160442BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK442

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

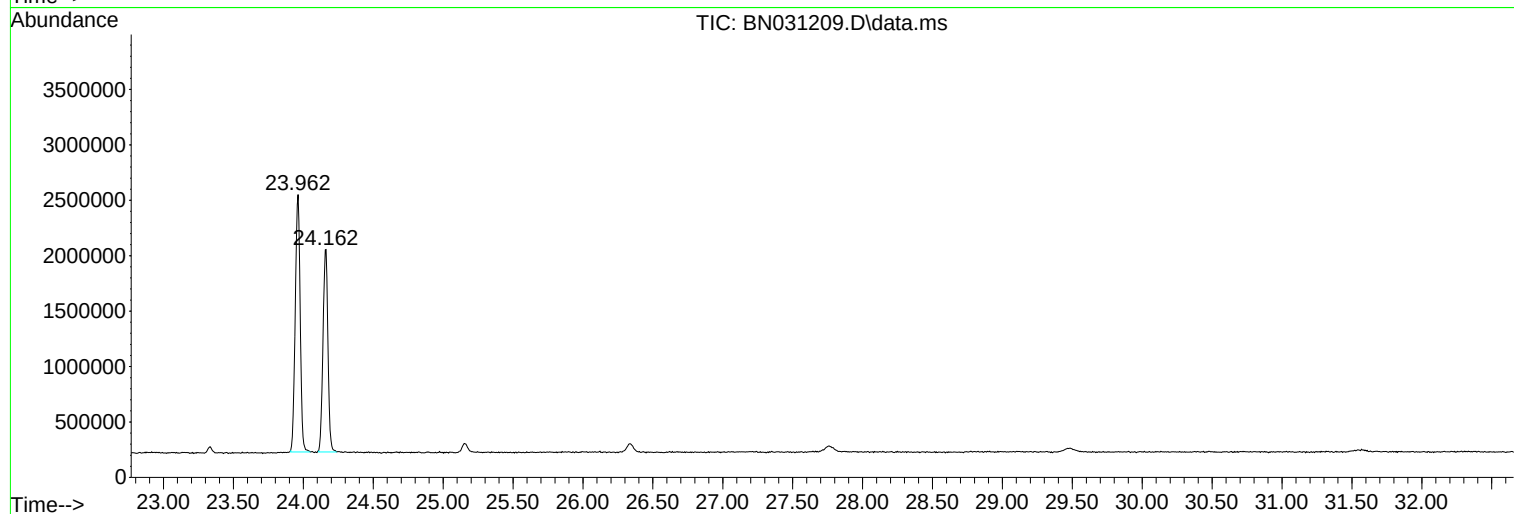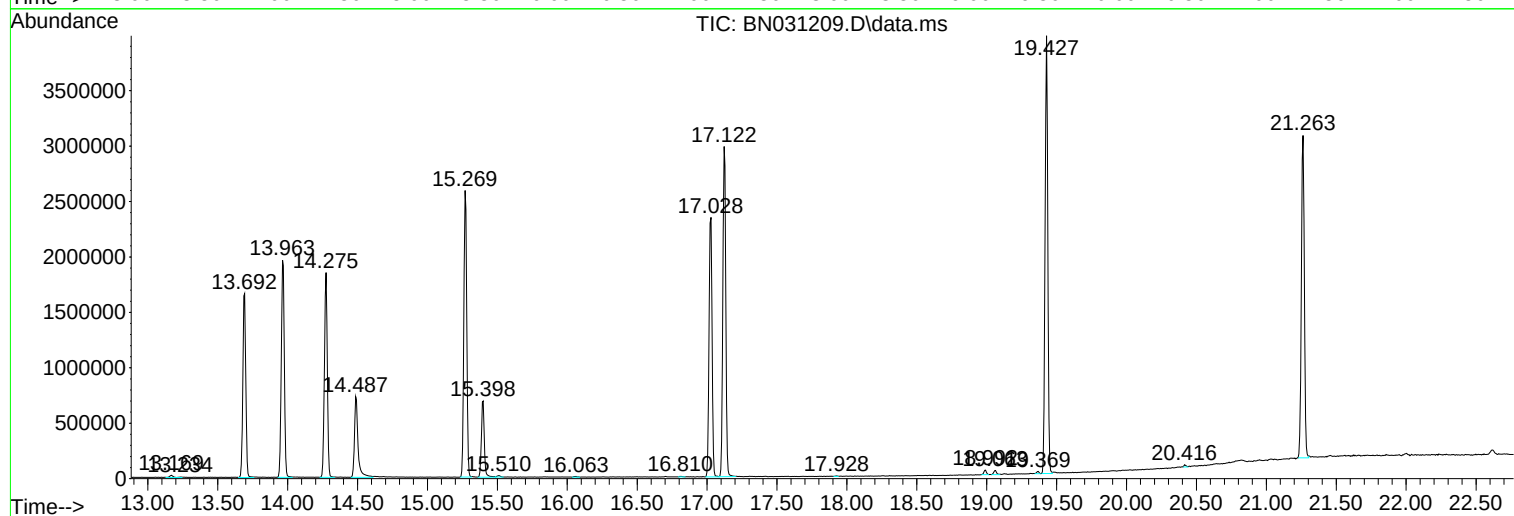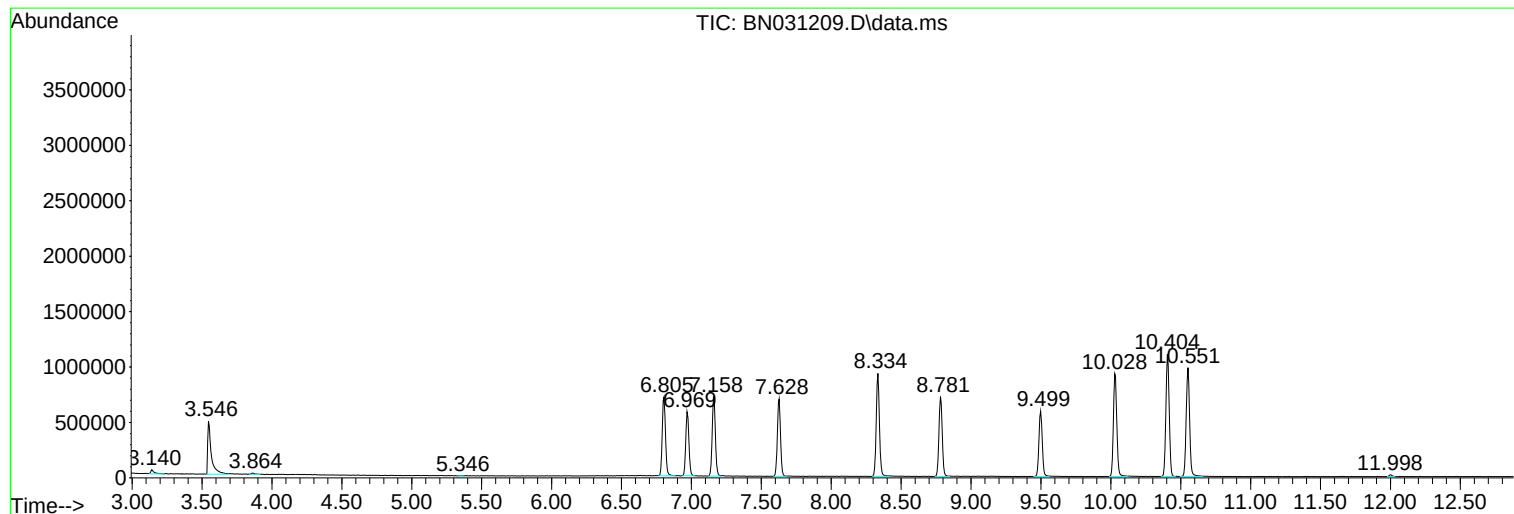

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031209.D
Acq On : 25 Apr 2024 05:27
Operator : MA/JU
Sample : PB160442BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK442

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042424\
Data File : BN031209.D
Acq On : 25 Apr 2024 05:27
Operator : MA/JU
Sample : PB160442BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK442

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------