

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042519\
 Data File : BN005294.D
 Acq On : 25 Apr 2019 23:34
 Operator : JU/SJ
 Sample : K2481-17
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 26 03:00:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	490976	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2147450	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1357067	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	3167468	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	3272065	20.00	ng/ul	-0.02
85) Perylene-d12	23.41	264	3740243	20.00	ng/ul	-0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	67438	6.63	ng/uL	0.00
5) Phenol-d5	6.78	99	1409113	36.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	844668	35.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1114121	37.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1146625	38.04	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	587919	44.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	661377	49.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1165330	37.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1585302	50.05	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3864553	39.23	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	4671984	38.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	678495	43.62	ng/ul	0.00
57) Fluorene-d10	15.23	176	3249645	39.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	583554	40.96	ng/ul	0.00
70) Anthracene-d10	17.08	188	5086787	38.31	ng/ul	0.00
78) Pyrene-d10	19.39	212	5854095	34.97	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.28	264	6491854	39.72	ng/ul	-0.02

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.29	70	28722	1.113	ng/ul#	1
44) Dimethylphthalate	13.69	163	768836	7.833	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042519\
Data File : BN005294.D
Acq On : 25 Apr 2019 23:34
Operator : JU/SJ
Sample : K2481-17
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 26 03:00:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

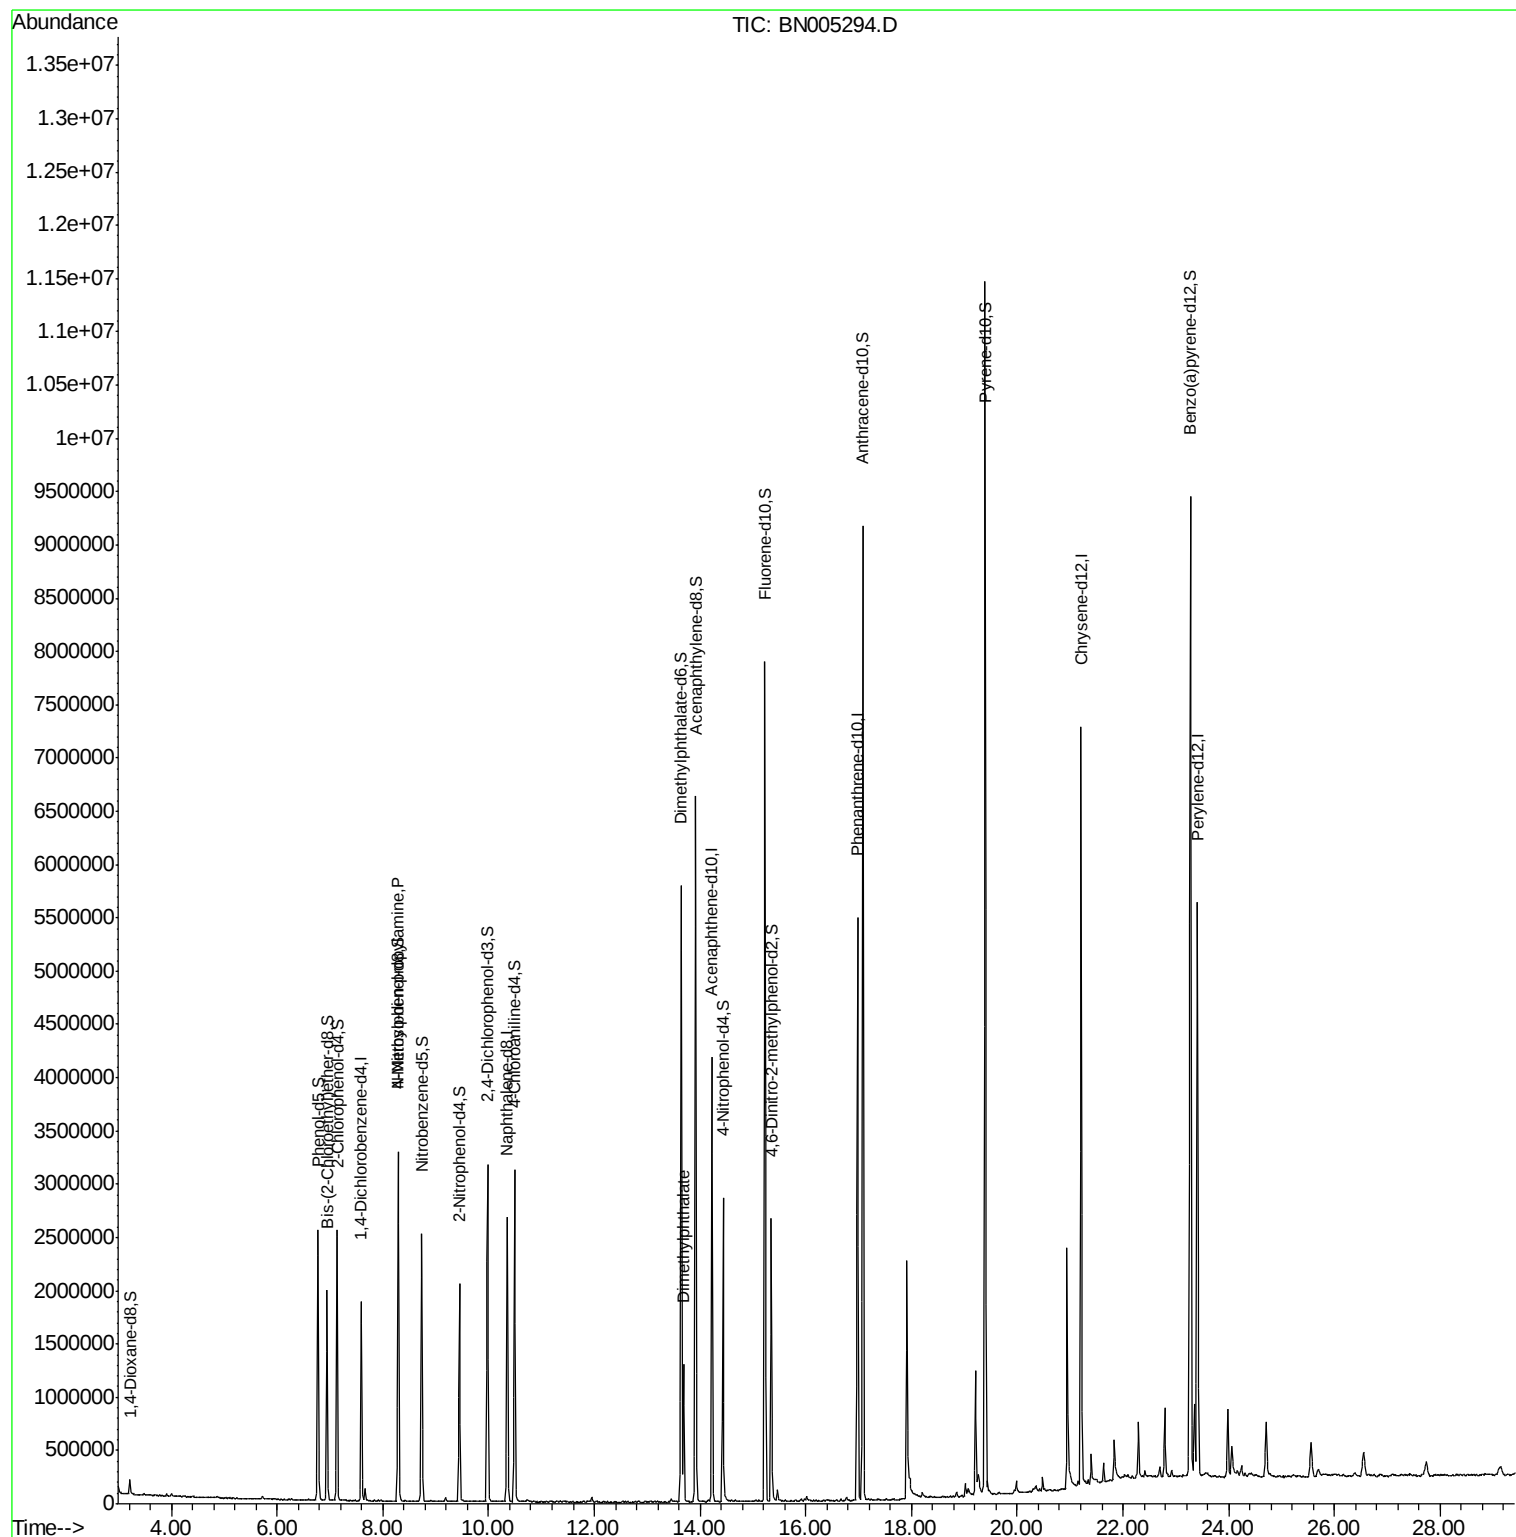

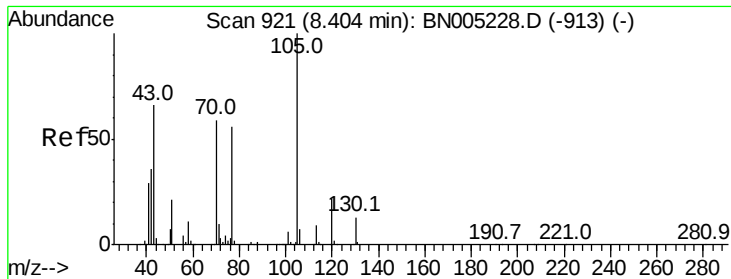

#15

N-Nitroso-di-n-propylamine

Concen: 1.113 ng/ul

RT: 8.29 min Scan# 902

Delta R.T. -0.11 min

Lab File: BN005294.D

Acq: 25 Apr 2019 23:34

Instrument :

BNA_N

ClientSampled :

Tot Ion: 70 Resp: 28722





Ion Ratio Lower Upper

70 100

42 385.0 53.8 80.8#

101 0.0 7.7 11.5#

130 0.0 15.0 22.4#

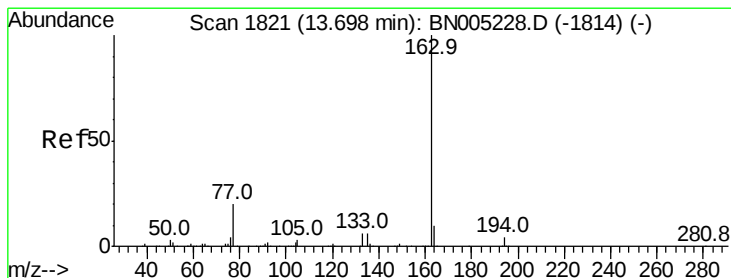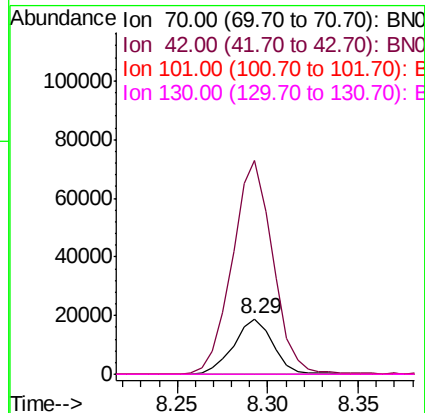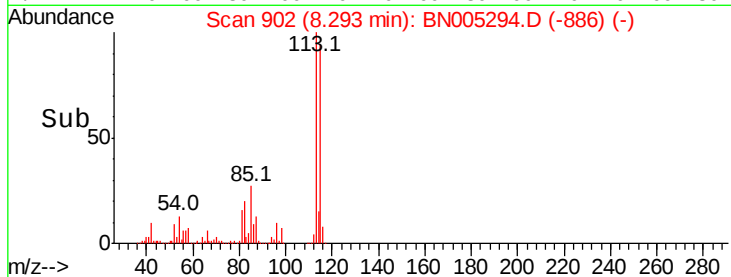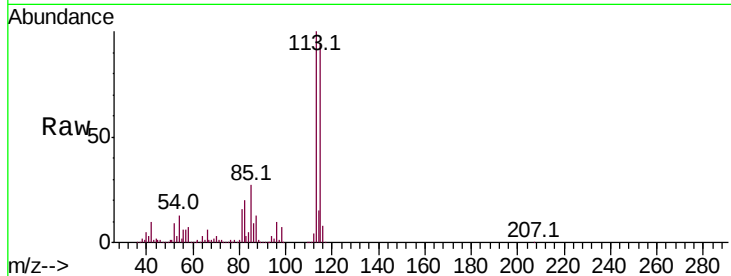

#44

Dimethylphthalate

Concen: 7.833 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005294.D

Acq: 25 Apr 2019 23:34

Tgt Ion:163 Resp: 768836

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 9.6 8.1 12.1

