

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042519\
 Data File : BN005297.D
 Acq On : 26 Apr 2019 01:17
 Operator : JU/SJ
 Sample : K2481-23
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 26 03:00:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	486310	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2218867	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1434122	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	3454137	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	3474383	20.00	ng/ul	-0.02
85) Perylene-d12	23.41	264	3826309	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	64804	6.43	ng/uL	0.00
5) Phenol-d5	6.78	99	1407532	36.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	860670	36.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1116556	38.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1192955	39.96	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	613806	44.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	687038	49.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	1209996	38.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1701667	51.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	4341965	41.71	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	5107718	39.95	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	674119	41.01	ng/ul	0.00
57) Fluorene-d10	15.23	176	3588083	41.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	605037	38.95	ng/ul	0.00
70) Anthracene-d10	17.08	188	5815213	40.16	ng/ul	0.00
78) Pyrene-d10	19.39	212	6719055	37.80	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	7049796	42.16	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	1023434	9.866	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042519\
Data File : BN005297.D
Acq On : 26 Apr 2019 01:17
Operator : JU/SJ
Sample : K2481-23
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 26 03:00:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

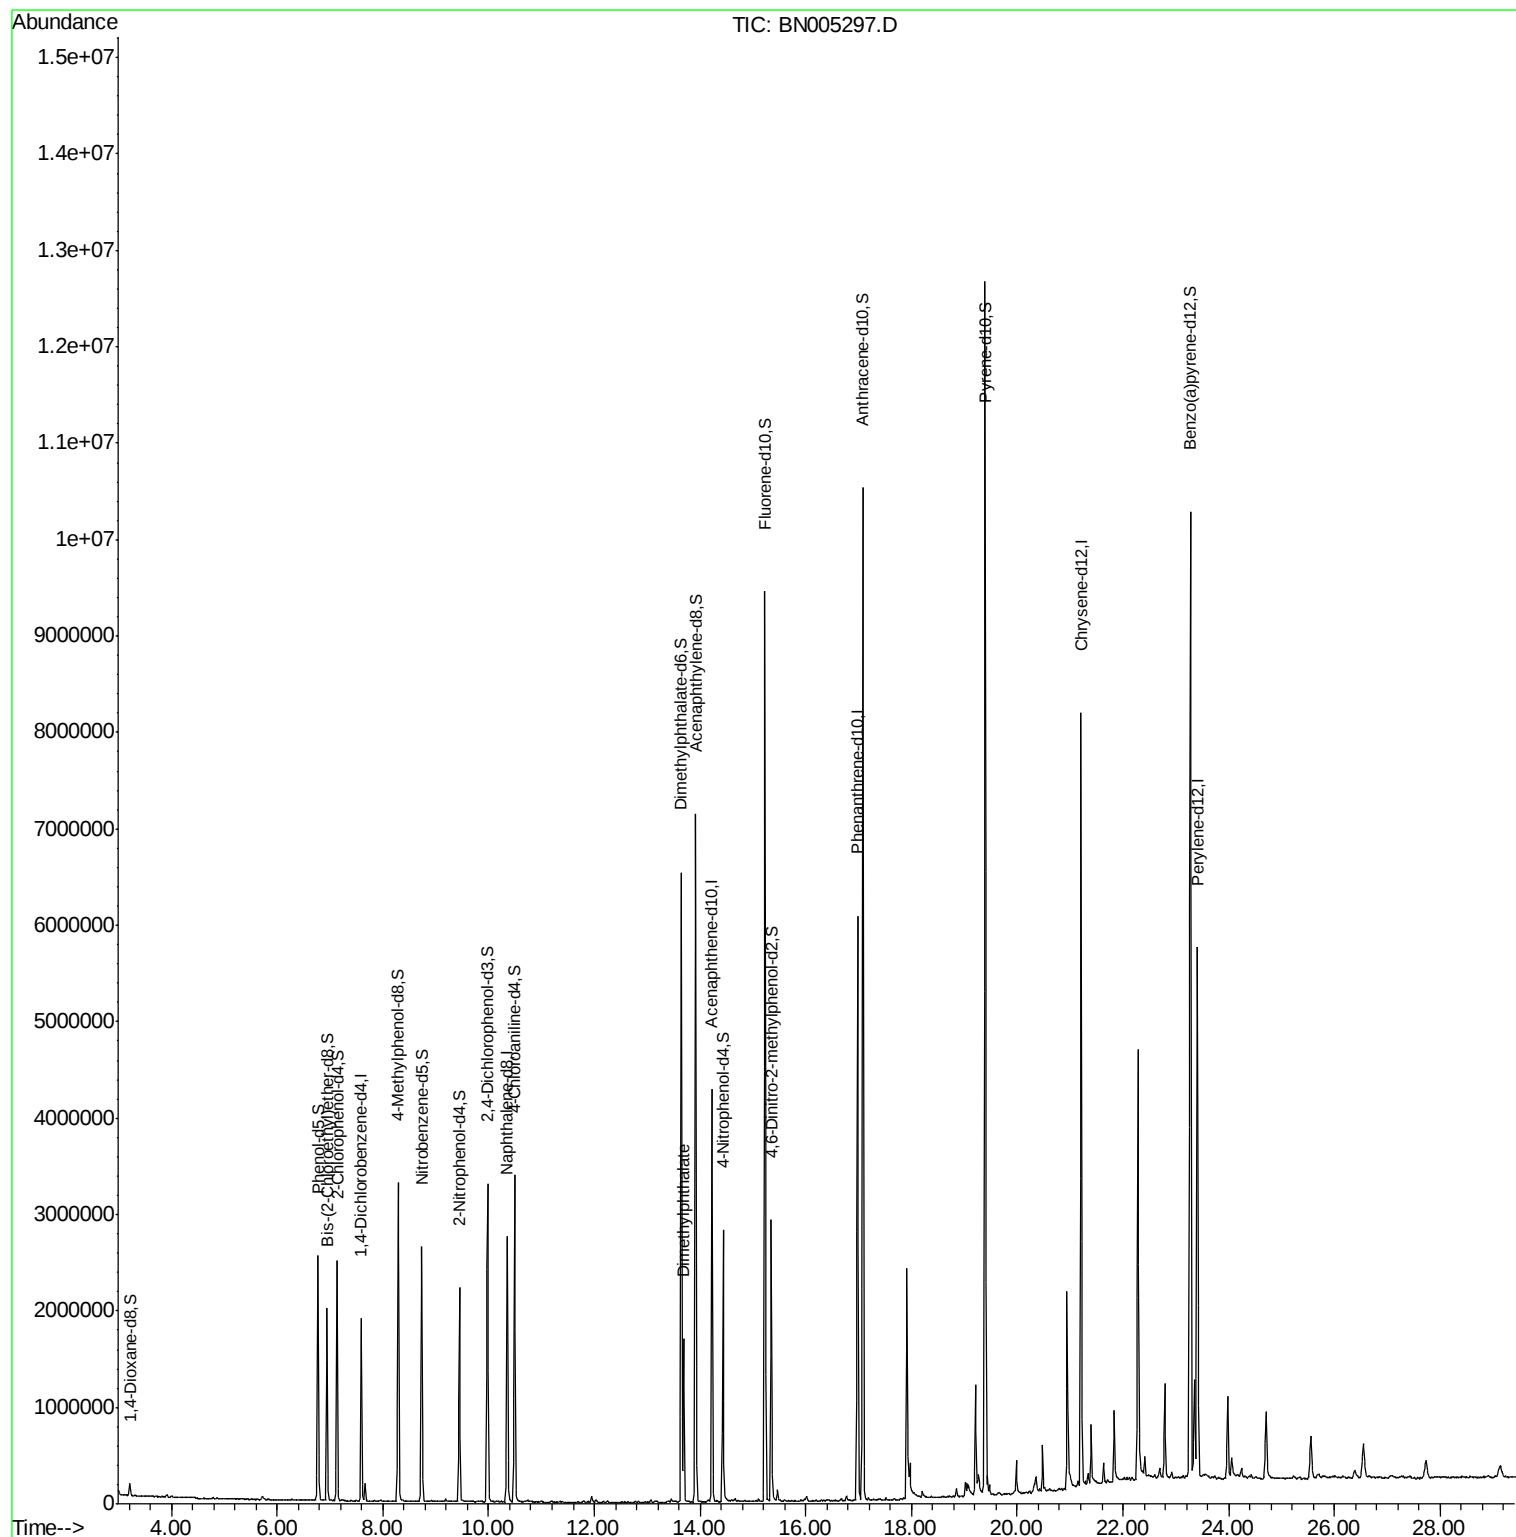

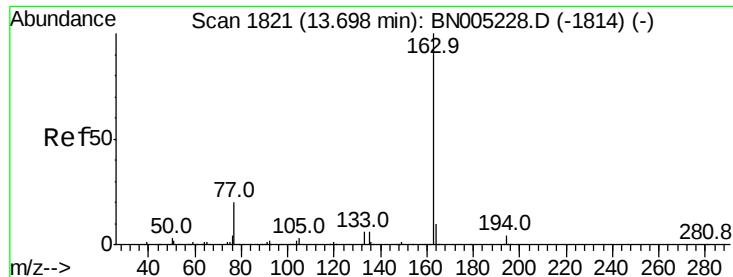

#44

Dimethylphthalate

Concen: 9.866 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005297.D

Acq: 26 Apr 2019 01:17

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 1023434

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 10.2 8.1 12.1

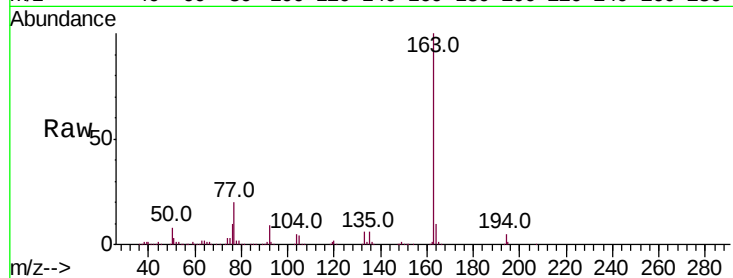

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

