

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042519\
 Data File : BN005307.D
 Acq On : 26 Apr 2019 07:03
 Operator : JU/SJ
 Sample : K2481-11 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 GAHW4

Manual Integrations
 APPROVED

Sohil
 4/26/2019 6:22:02 PM

Quant Time: Apr 26 07:55:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	507739	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2168191	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1286694	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2923578	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	2776633	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2604355	20.00	ng/ul	-0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	3122	0.30	ng/uL	0.00
5) Phenol-d5	6.78	99	71248	1.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	45939	1.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	57903	1.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	59551	1.91	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	30810	2.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	30485	2.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	63155	2.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	45795	1.43	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	222054	2.38	ng/ul	-0.01
46) Acenaphthylene-d8	13.92	160	268158	2.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	23254	1.58	ng/ul	0.00
57) Fluorene-d10	15.23	176	196710	2.51	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	17131	1.30	ng/ul	0.00
70) Anthracene-d10	17.07	188	316234	2.58	ng/ul	-0.01
78) Pyrene-d10	19.39	212	341782	2.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	268261	2.36	ng/ul	-0.04

Target Compounds

					Qvalue
47) Acenaphthylene	13.95	152	832378	7.383 ng/ul	99
71) Anthracene	17.11	178	258168	1.780 ng/ul	97
87) Benzo(b)fluoranthene	22.76	252	523517m	3.576 ng/ul	
90) Benzo(a)pyrene	23.31	252	740305	5.380 ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.58	276	338810	2.227 ng/ul	97
93) Benzo(g,h,i)perylene	26.24	276	273569	2.175 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042519\
Data File : BN005307.D
Acq On : 26 Apr 2019 07:03
Operator : JU/SJ
Sample : K2481-11 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
GAHW4

Manual Integrations
APPROVED

Sohil
4/26/2019 6:22:02 PM

Quant Time: Apr 26 07:55:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

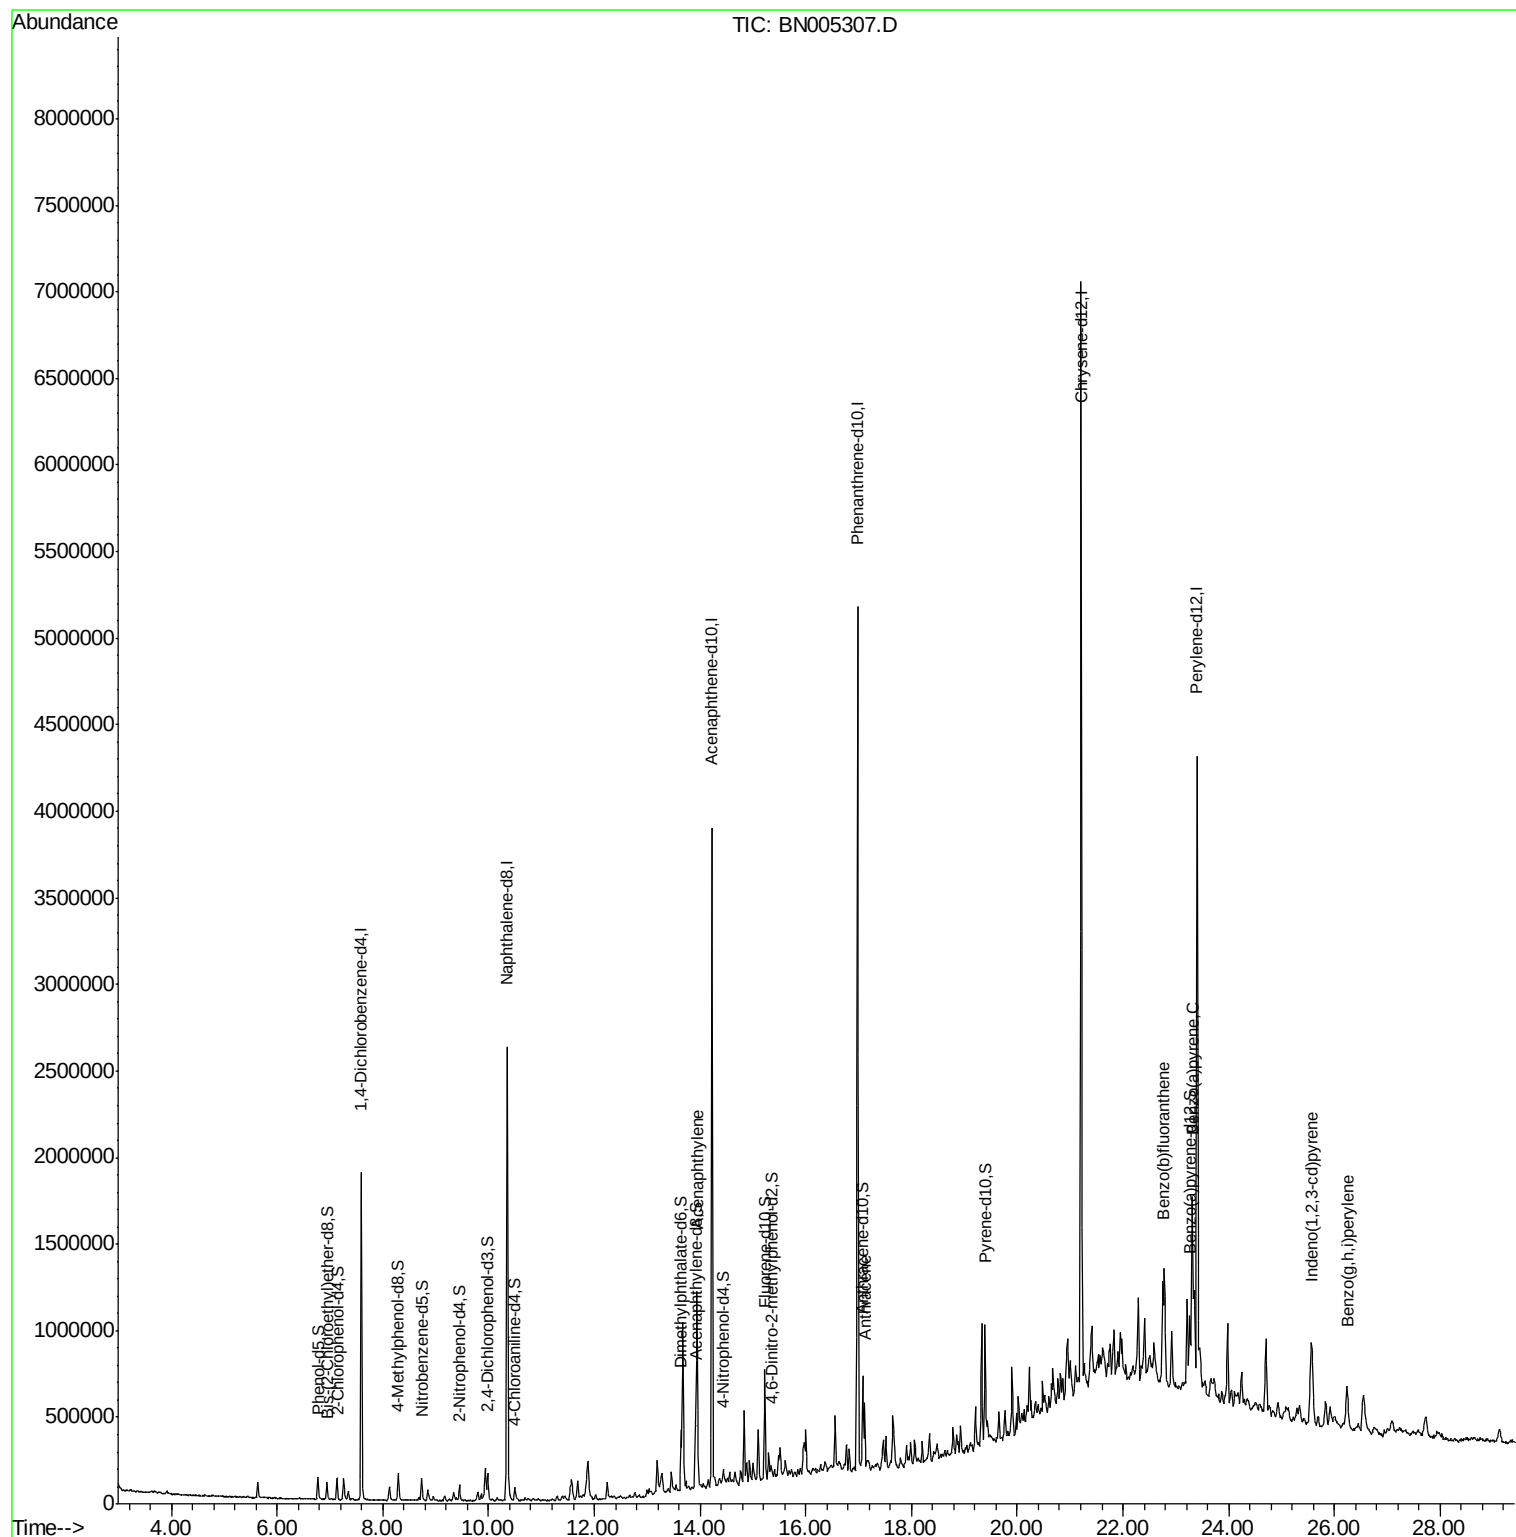

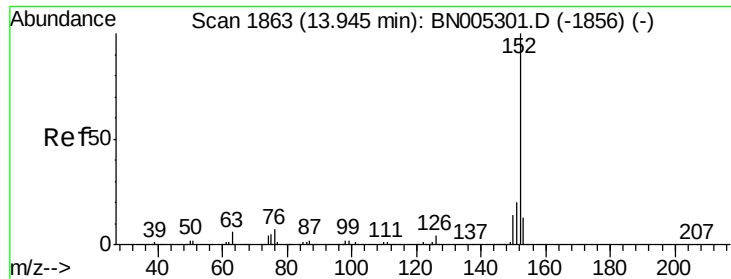

#47

Acenaphthylene

Concen: 7.383 ng/ul

RT: 13.95 min Scan# 1863

Delta R.T. -0.01 min

Lab File: BN005307.D

Acq: 26 Apr 2019 07:03

Instrument :

BNA_N





ClientSampleId :

GAHW4

Tgt Ion:	152	Resp:	832378
Ion Ratio	Lower	Upper	
152	100		
151	19.8	15.8	23.8
153	13.3	9.8	14.8

Manual Integrations
APPROVED

Sohil
4/26/2019 6:22:02 PM

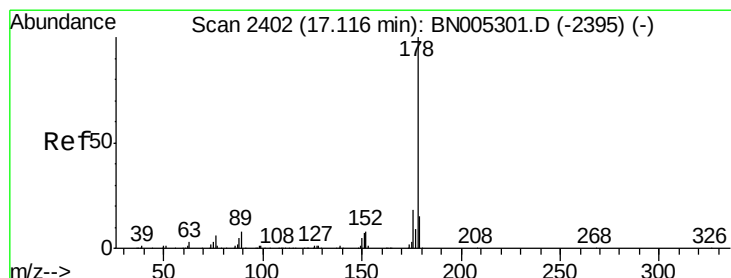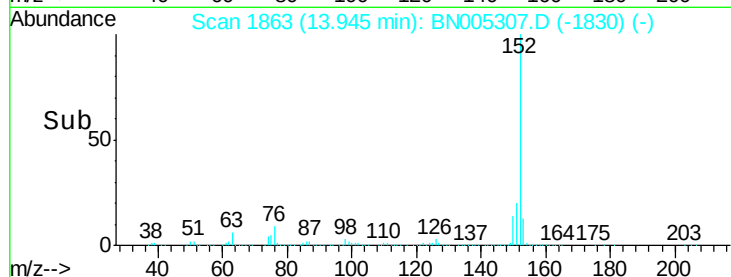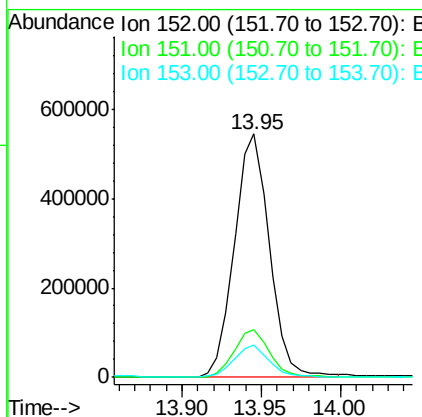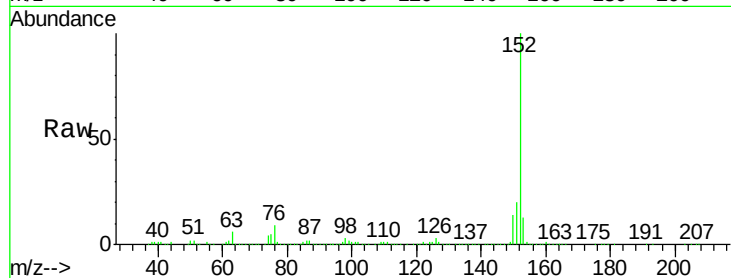

#71

Anthracene

Concen: 1.780 ng/ul




RT: 17.11 min Scan# 2401


Delta R.T. -0.01 min

Lab File: BN005307.D

Acq: 26 Apr 2019 07:03

Tgt Ion:	178	Resp:	258168
Ion Ratio	Lower	Upper	
178	100		
179	16.3	12.3	18.5
176	17.2	15.1	22.7

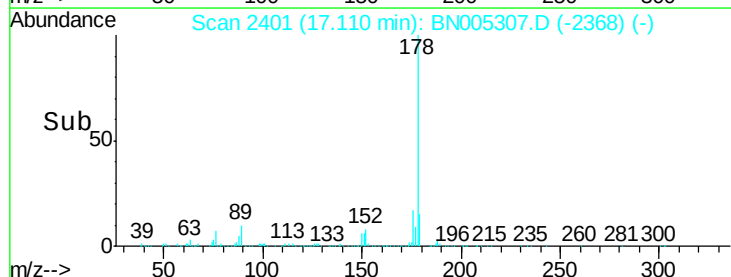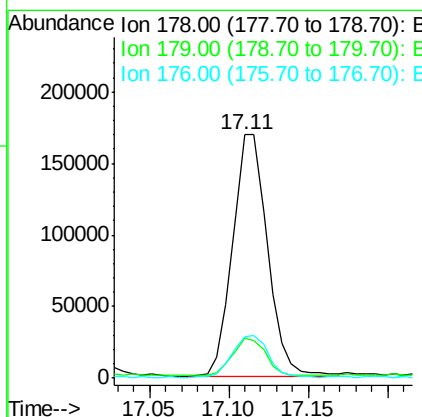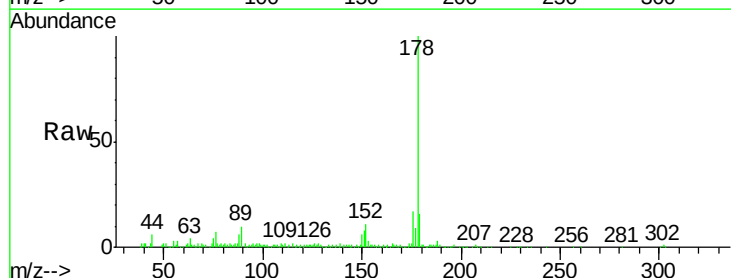

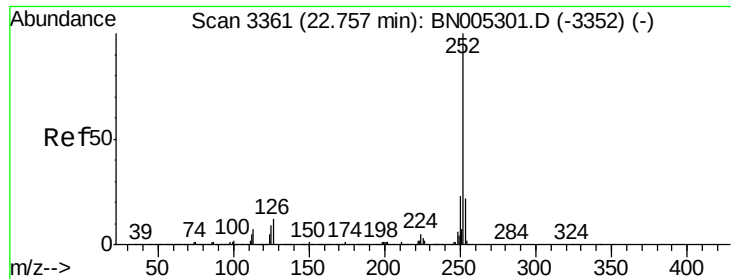





#87
Benzo(b)fluoranthene
Concen: 3.576 ng/ul m
RT: 22.76 min Scan# 3361
Delta R.T. -0.03 min
Lab File: BN005307.D
Acq: 26 Apr 2019 07:03

Instrument :
BNA_N
ClientSampleId :
GAHW4

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.4	17.7	26.5
125	10.8	8.4	12.6




Manual Integrations
APPROVED


Sohil
4/26/2019 6:22:02 PM

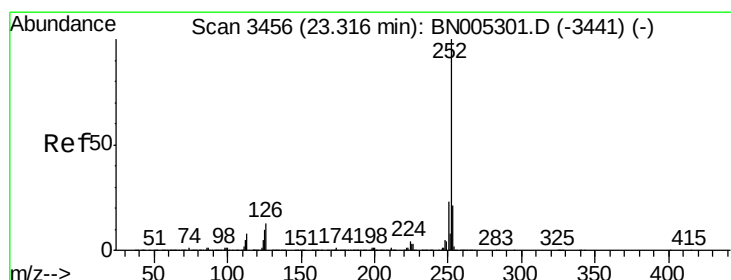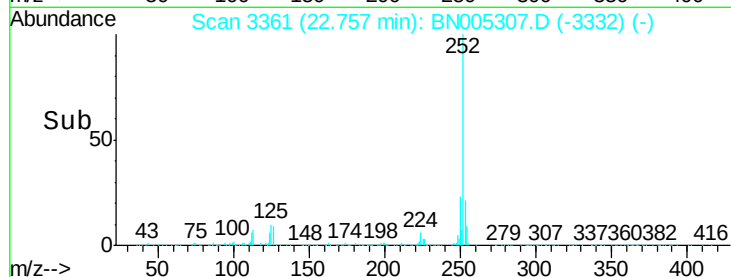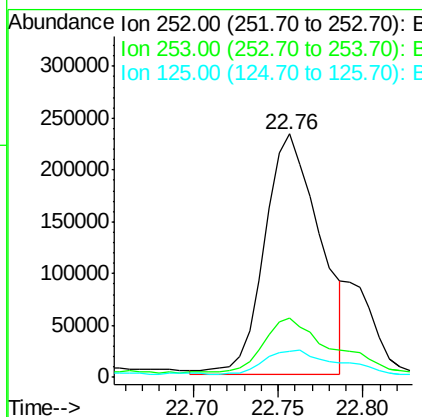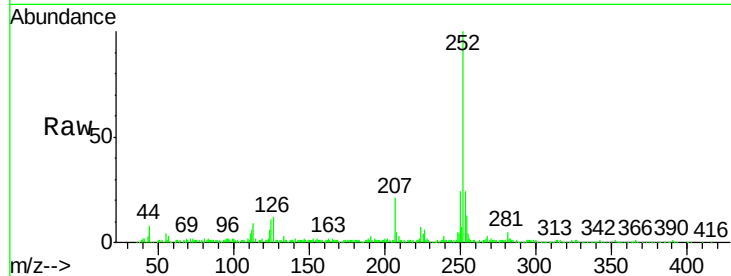

#90
Benzo(a)pyrene
Concen: 5.380 ng/ul
RT: 23.31 min Scan# 3455
Delta R.T. -0.04 min
Lab File: BN005307.D
Acq: 26 Apr 2019 07:03

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.3	25.9
125	10.8	8.6	13.0

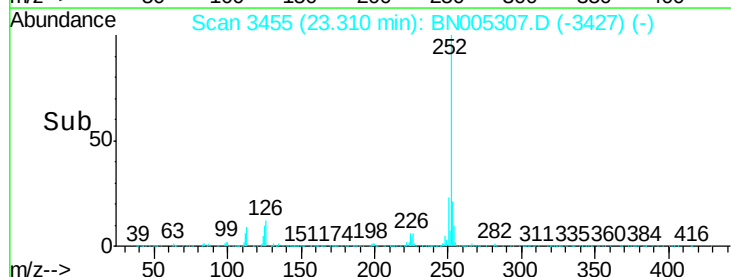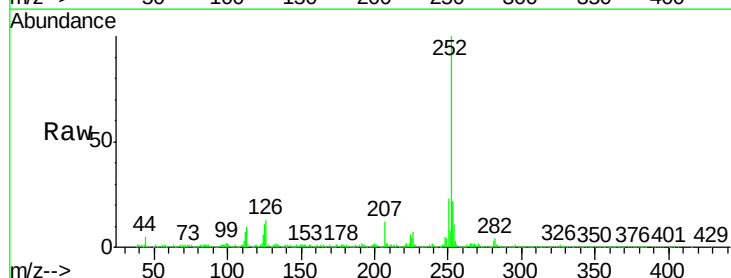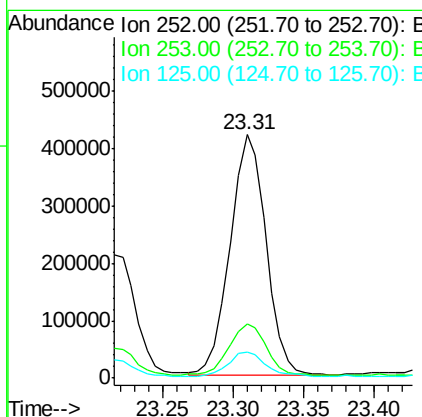

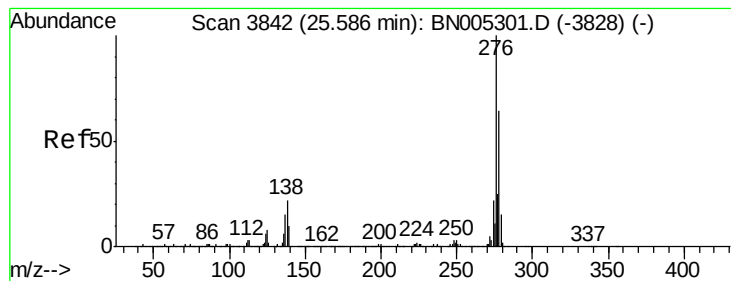

#91

Indeno(1,2,3-cd)pyrene

Concen: 2.227 ng/ul

RT: 25.58 min Scan# 3841

Delta R.T. -0.05 min

Lab File: BN005307.D


Acq: 26 Apr 2019 07:03

Instrument :

BNA_N

ClientSampled :

GAHW4

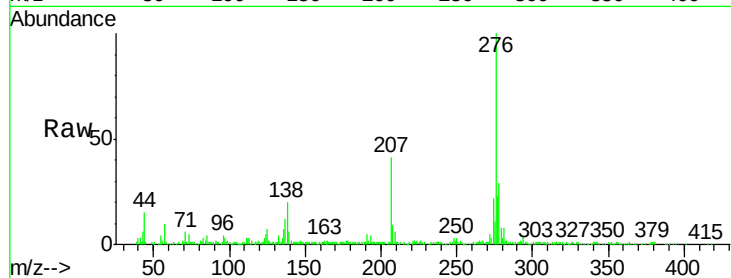

Tgt Ion: 276 Resp: 338810

Ion Ratio Lower Upper




276 100

138 20.4 17.9 26.9

277 23.3 19.7 29.5

Manual Integrations
APPROVED

Sohil
4/26/2019 6:22:02 PM

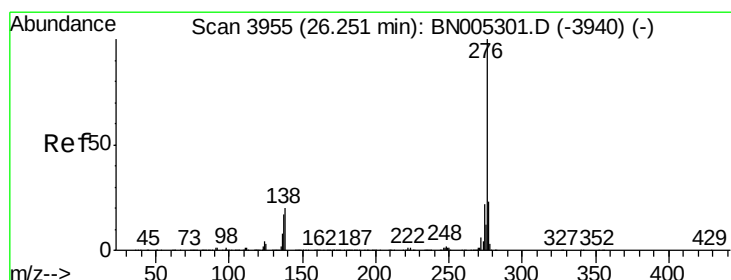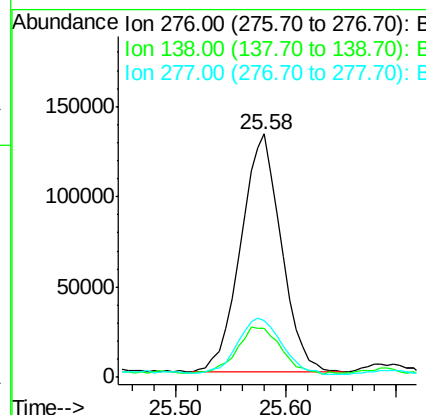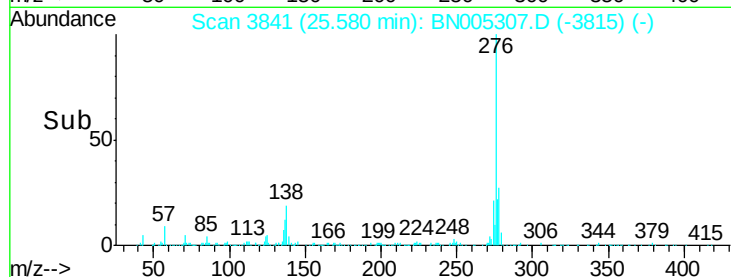

#93

Benzo(g,h,i)perylene

Concen: 2.175 ng/ul

RT: 26.24 min Scan# 3954

Delta R.T. -0.05 min

Lab File: BN005307.D

Acq: 26 Apr 2019 07:03

Tgt Ion: 276 Resp: 273569

Ion Ratio Lower Upper

276 100

138 19.6 16.7 25.1

277 23.7 18.2 27.2

