




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031258.D
Acq On : 27 Apr 2024 00:24
Operator : MA/JU
Sample : P2161-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORD7

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:03:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 22:57:25 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/29/2024
Supervised By :mohammad ahmed 04/29/2024

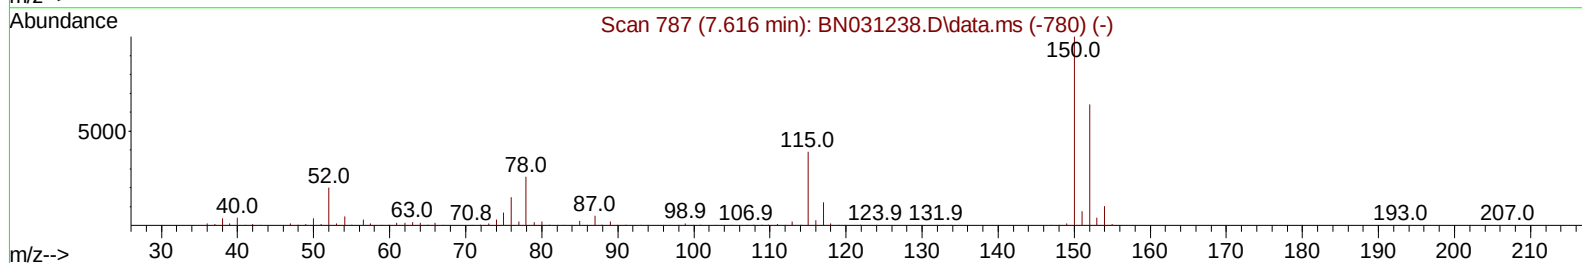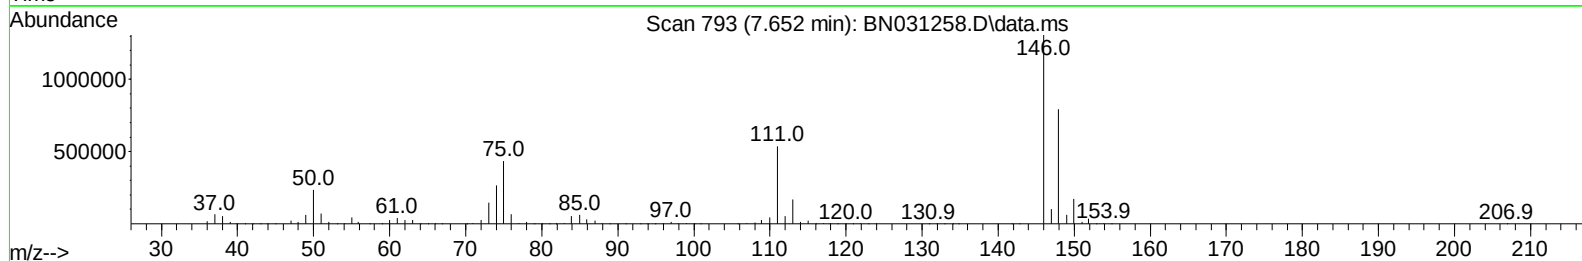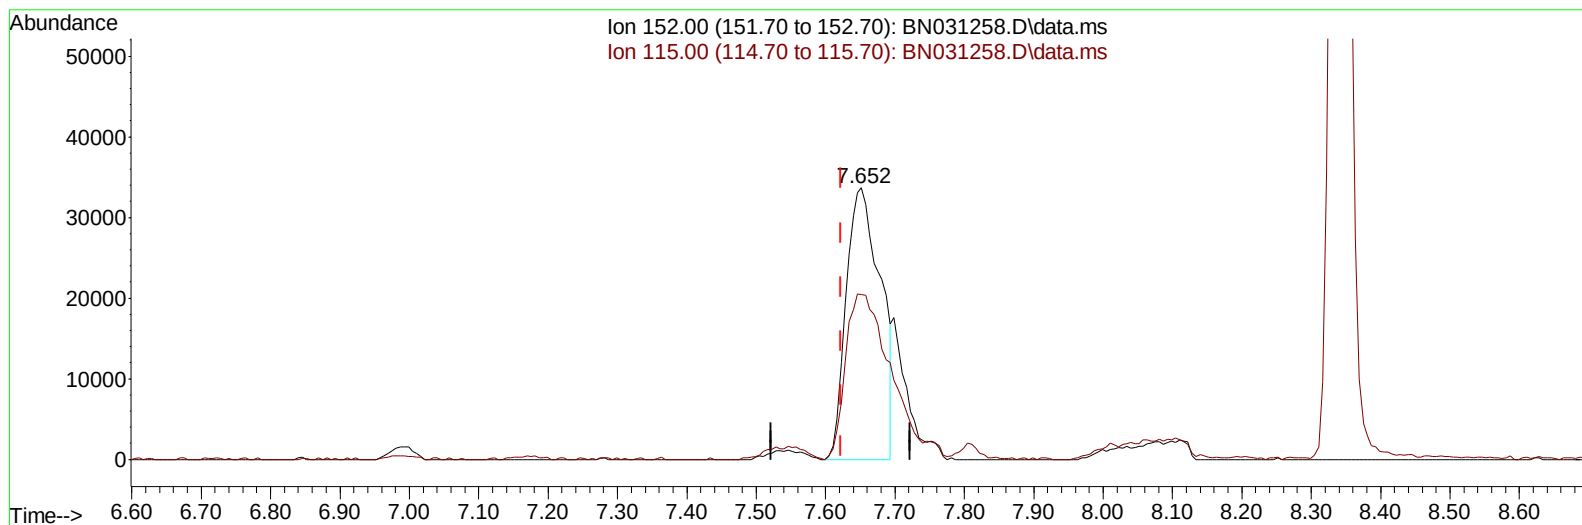

TIC: BN031258.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.652min (+ 0.030) 20.00 ng/u1

response 115623

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	58.40	60.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031258.D
Acq On : 27 Apr 2024 00:24
Operator : MA/JU
Sample : P2161-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CORD7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/29/2024
Supervised By :mohammad ahmed 04/29/2024

Quant Time: Apr 27 01:03:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 22:57:25 2024
Response via : Initial Calibration

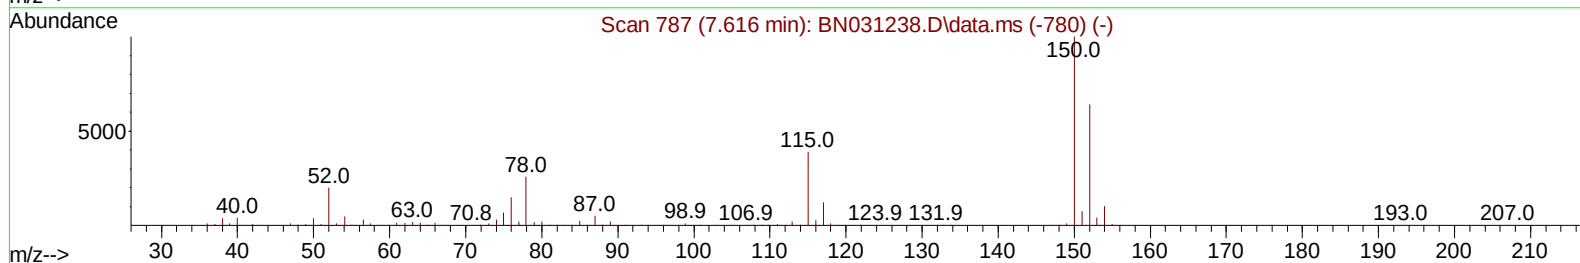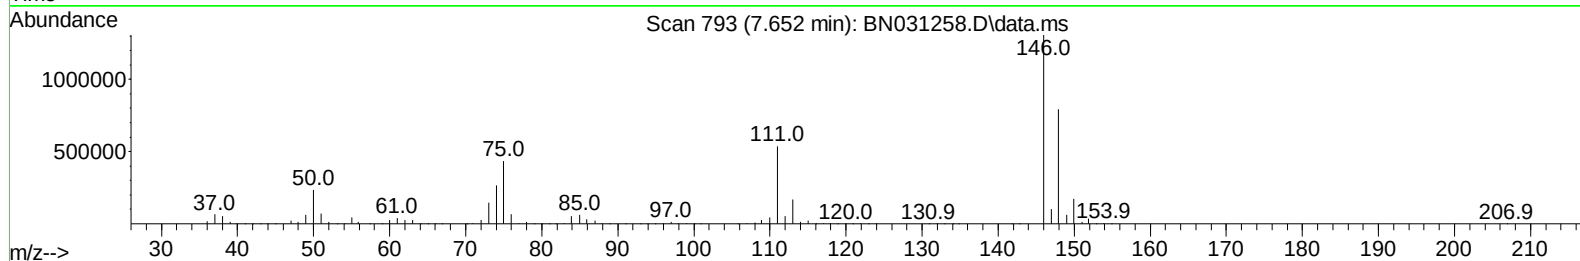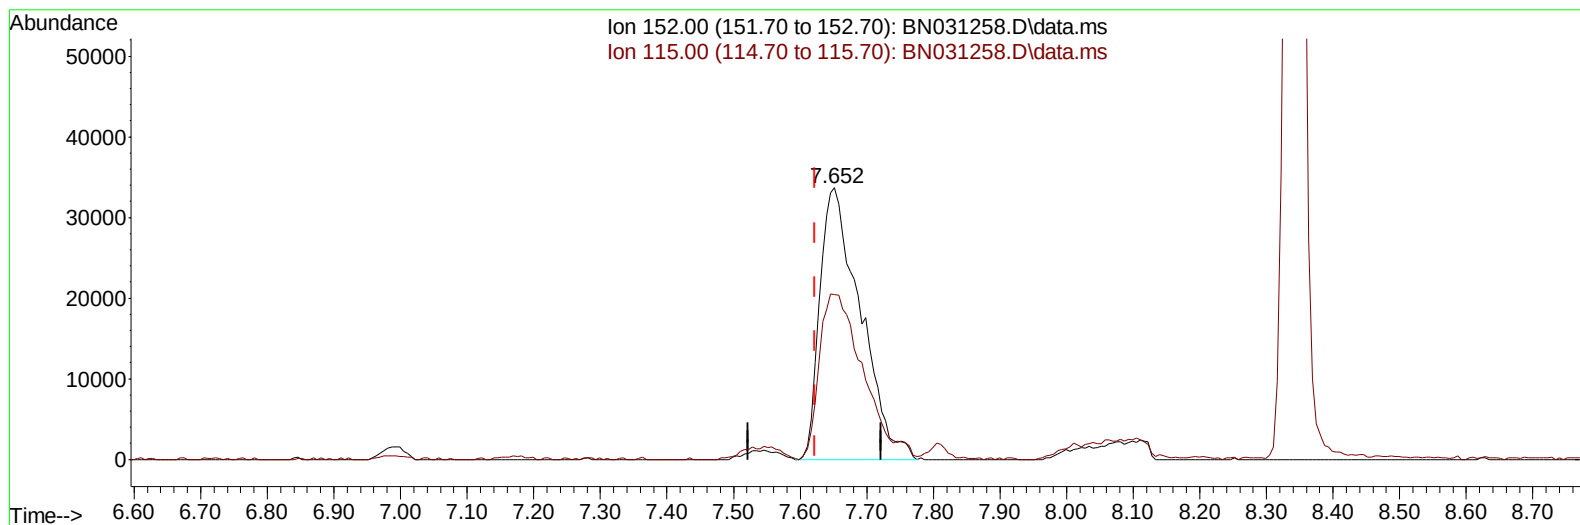

TIC: BN031258.D\data.ms

(1) 1,4-Dichlorobenzene-d4 (I)

7.652min (+ 0.030) 20.00 ng/ul m

response 142172

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	58.40	60.75
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031258.D
 Acq On : 27 Apr 2024 00:24
 Operator : MA/JU
 Sample : P2161-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CORD7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/29/2024
 Supervised By :mohammad ahmed 04/29/2024

Quant Time: Apr 27 01:24:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 22:57:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	142172m	20.000	ng/uL	0.03
20) Naphthalene-d8	10.434	136	1067125	20.000	ng/uL	0.03
38) Acenaphthene-d10	14.269	164	685976	20.000	ng/uL	0.00
64) Phenanthrene-d10	17.022	188	1443994	20.000	ng/uL	0.00
79) Chrysene-d12	21.257	240	1321022	20.000	ng/uL	0.00
88) Perylene-d12	24.151	264	1230073	20.000	ng/uL	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	32735	10.757	ng/uL	0.00
4) Pyridine-d5	3.552	84	244060	27.849	ng/uL	0.00
7) Phenol-d5	6.805	99	227208	18.945	ng/uL	0.00
9) Bis-(2-Chloroethyl)eth...	6.993	67	616818	88.398	ng/uL	0.02
11) 2-Chlorophenol-d4	7.169	132	656406	70.294	ng/uL	0.01
15) 4-Methylphenol-d8	8.340	113	398633	39.523	ng/uL	0.00
21) Nitrobenzene-d5	8.793	128	427803	55.796	ng/uL	0.01
24) 2-Nitrophenol-d4	9.505	143	457773	57.438	ng/uL	0.01
28) 2,4-Dichlorophenol-d3	10.040	165	716350	45.578	ng/uL	0.01
31) 4-Chloroaniline-d4	10.563	131	981104	39.946	ng/uL	0.02
46) Dimethylphthalate-d6	13.693	166	2415125	50.594	ng/uL	0.00
49) Acenaphthylene-d8	13.963	160	2809931	51.946	ng/uL	0.00
54) 4-Nitrophenol-d4	14.487	143	97103	9.746	ng/uL	0.00
60) Fluorene-d10	15.269	176	2038268	49.050	ng/uL	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	361529	49.625	ng/uL	0.00
73) Anthracene-d10	17.122	188	3075592	49.140	ng/uL	0.00
81) Pyrene-d10	19.428	212	3651159	56.246	ng/uL	0.00
92) Benzo(a)pyrene-d12	23.963	264	3260022	55.888	ng/uL	0.00
Target Compounds						
						Qvalue
12) 2-Chlorophenol	7.205	128	19982	2.059	ng/uL	91
30) Naphthalene	10.481	128	93321	1.687	ng/uL	98
39) 1,2,4,5-Tetrachloroben...	12.446	216	1513563	84.322	ng/uL	98
75) 1,2,3,4-Tetrachloroben...	13.069	216	2527996	149.256	ng/uL	98
76) Pentachlorobenzene	14.587	250	46364	2.651	ng/uL	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031258.D
Acq On : 27 Apr 2024 00:24
Operator : MA/JU
Sample : P2161-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0RD7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/29/2024
Supervised By :mohammad ahmed 04/29/2024

Quant Time: Apr 27 01:24:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 22:57:25 2024
Response via : Initial Calibration

