

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031250.D
 Acq On : 26 Apr 2024 17:46
 Operator : MA/JU
 Sample : P2161-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R89

Quant Time: Apr 26 18:25:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 19 22:56:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	282239	20.000	ng/ul	-0.02
20) Naphthalene-d8	10.405	136	1269509	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.269	164	833560	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.022	188	1700653	20.000	ng/ul	-0.01
79) Chrysene-d12	21.257	240	1369606	20.000	ng/ul	-0.01
88) Perylene-d12	24.157	264	1251975	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	33167	5.490	ng/uL	0.00
4) Pyridine-d5	3.546	84	214451	12.326	ng/ul	0.00
7) Phenol-d5	6.799	99	192283	8.076	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	6.969	67	594989	42.953	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.158	132	603359	32.547	ng/ul	-0.01
15) 4-Methylphenol-d8	8.334	113	382514	19.104	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	430597	47.208	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.493	143	457178	48.218	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.028	165	713047	38.136	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.552	131	961703	32.914	ng/ul	-0.01
46) Dimethylphthalate-d6	13.693	166	2648788	45.665	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	2907990	44.241	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.493	143	84482	6.978	ng/ul	0.00
60) Fluorene-d10	15.269	176	2189099	43.352	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.398	200	253951	29.598	ng/ul	0.00
73) Anthracene-d10	17.122	188	3253172	44.133	ng/ul	-0.01
81) Pyrene-d10	19.428	212	3790260	56.317	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	2979882	50.192	ng/ul	-0.02
Target Compounds						
35) 4-Chloro-3-methylphenol	11.699	107	48479	2.239	ng/ul	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031250.D
Acq On : 26 Apr 2024 17:46
Operator : MA/JU
Sample : P2161-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R89


Quant Time: Apr 26 18:25:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 19 22:56:25 2024
Response via : Initial Calibration

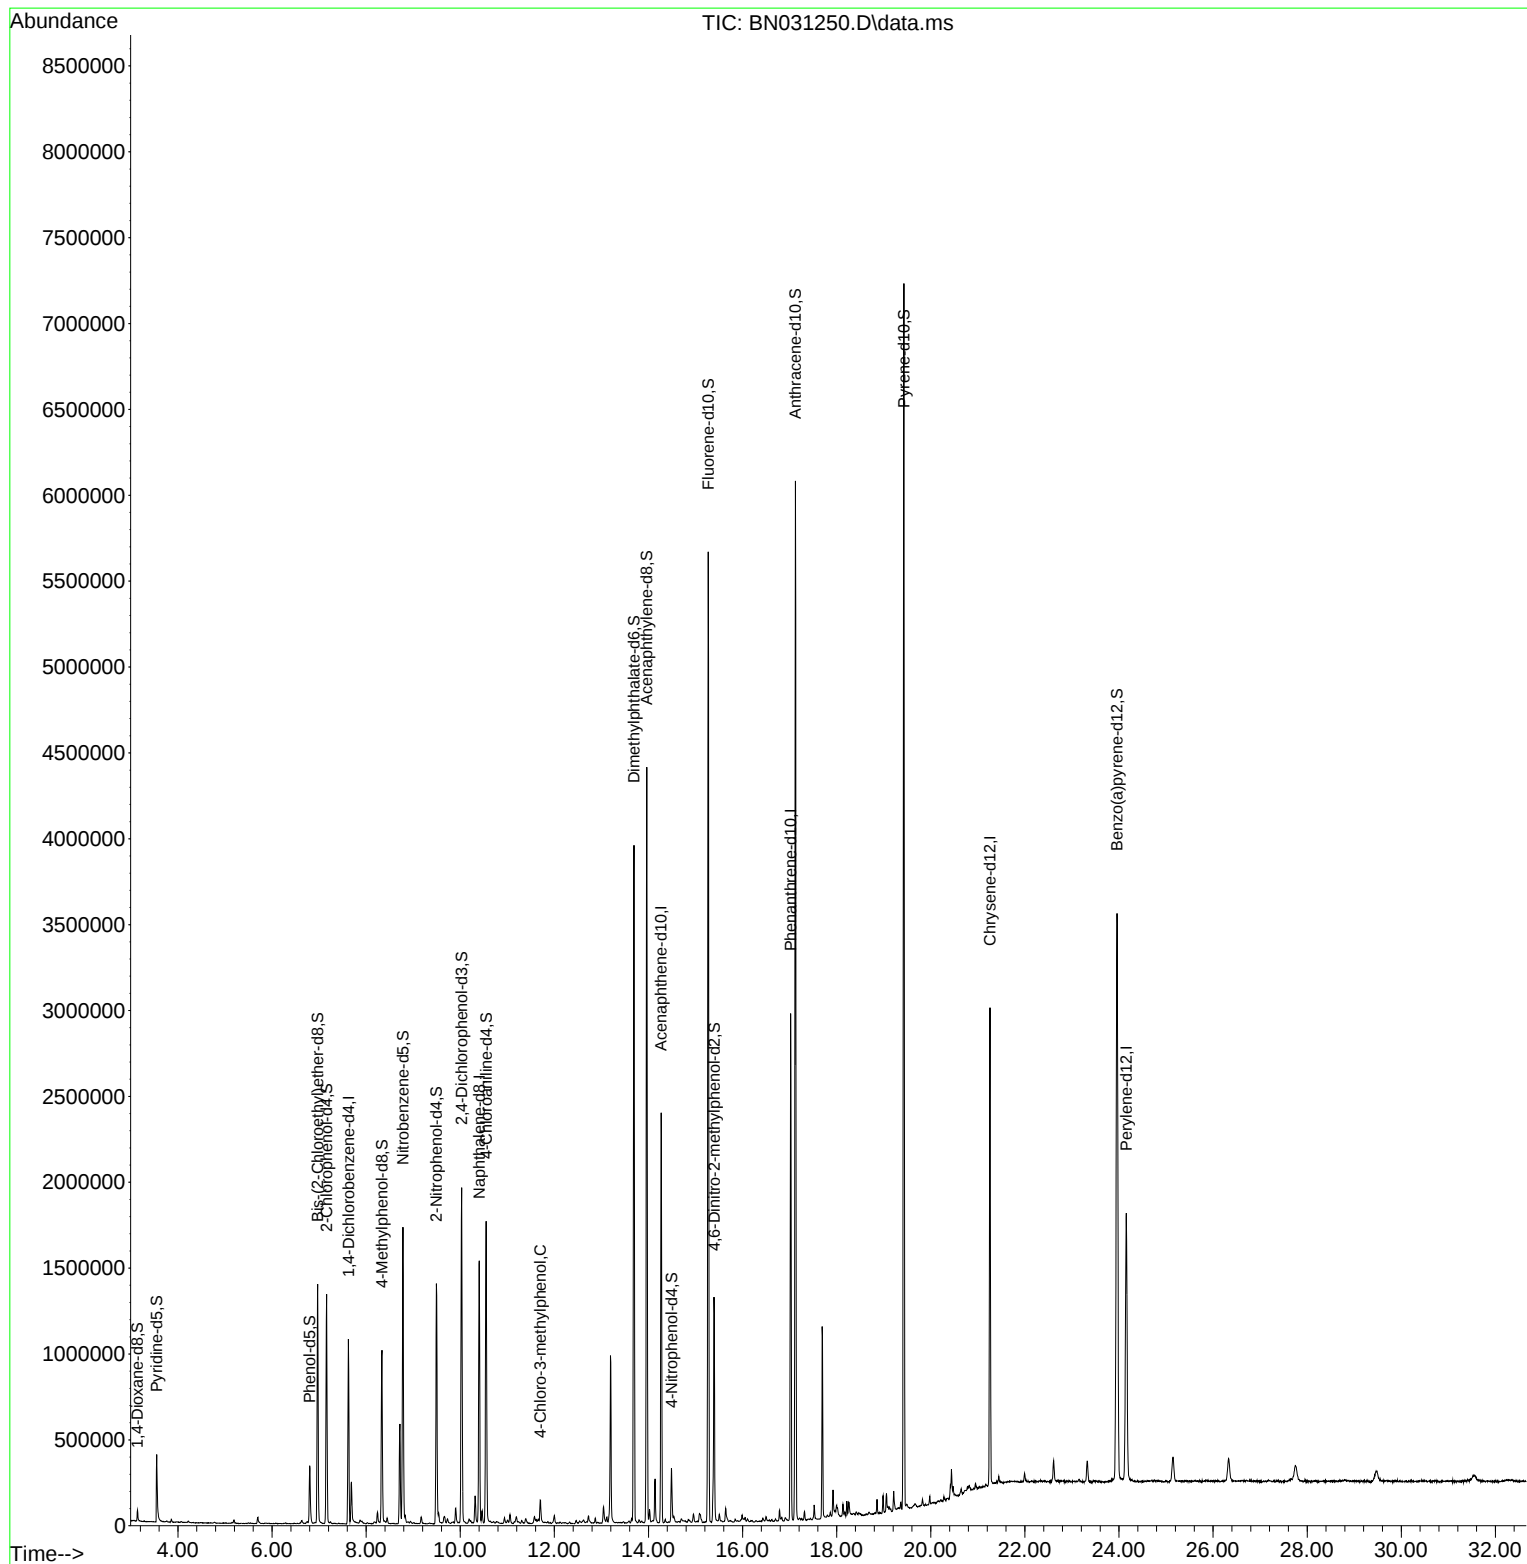

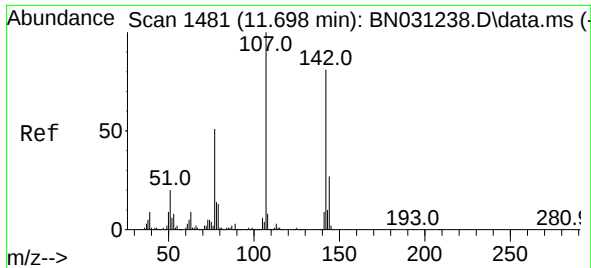

#35
 4-Chloro-3-methylphenol
 Concen: 2.239 ng/ul
 RT: 11.699 min Scan# 1481
 Delta R.T. -0.012 min
 Lab File: BN031250.D
 Acq: 26 Apr 2024 17:46

Instrument :
 BNA_N
 ClientSampleId :
 C0R89

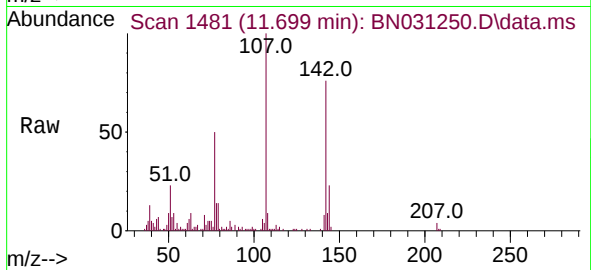

Tgt Ion:	107	Resp:	48479
Ion	Ratio	Lower	Upper
107	100		
144	23.2	20.6	31.0
142	76.4	67.4	101.2

