

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031255.D
 Acq On : 26 Apr 2024 22:23
 Operator : MA/JU
 Sample : P2280-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E08P1

Quant Time: Apr 26 23:13:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 26 22:57:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	278785	20.000	ng/ul	0.00
20) Naphthalene-d8	10.399	136	1224348	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	805356	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	1593498	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1124612	20.000	ng/ul	0.00
88) Perylene-d12	24.145	264	1068353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.140	96	25330	4.245	ng/uL	0.00
4) Pyridine-d5	3.552	84	104343	6.072	ng/ul	0.00
7) Phenol-d5	6.799	99	147489	6.271	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.964	67	425281	31.082	ng/ul	0.00
11) 2-Chlorophenol-d4	7.158	132	455648	24.884	ng/ul	0.00
15) 4-Methylphenol-d8	8.328	113	289290	14.627	ng/ul	0.00
21) Nitrobenzene-d5	8.781	128	306613	34.855	ng/ul	0.00
24) 2-Nitrophenol-d4	9.493	143	326969	35.757	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.028	165	510394	28.304	ng/ul	0.00
31) 4-Chloroaniline-d4	10.546	131	559882	19.868	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	1908016	34.046	ng/ul	0.00
49) Acenaphthylene-d8	13.963	160	2075646	32.684	ng/ul	0.00
54) 4-Nitrophenol-d4	14.493	143	58863	5.032	ng/ul	0.00
60) Fluorene-d10	15.269	176	1553254	31.837	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.393	200	275770	34.302	ng/ul	0.00
73) Anthracene-d10	17.122	188	2508032	36.313	ng/ul	0.00
81) Pyrene-d10	19.428	212	2559051	46.307	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.951	264	1933001	38.155	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.775	77	29488	2.554	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031255.D
Acq On : 26 Apr 2024 22:23
Operator : MA/JU
Sample : P2280-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E08P1


Quant Time: Apr 26 23:13:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 26 22:57:25 2024
Response via : Initial Calibration

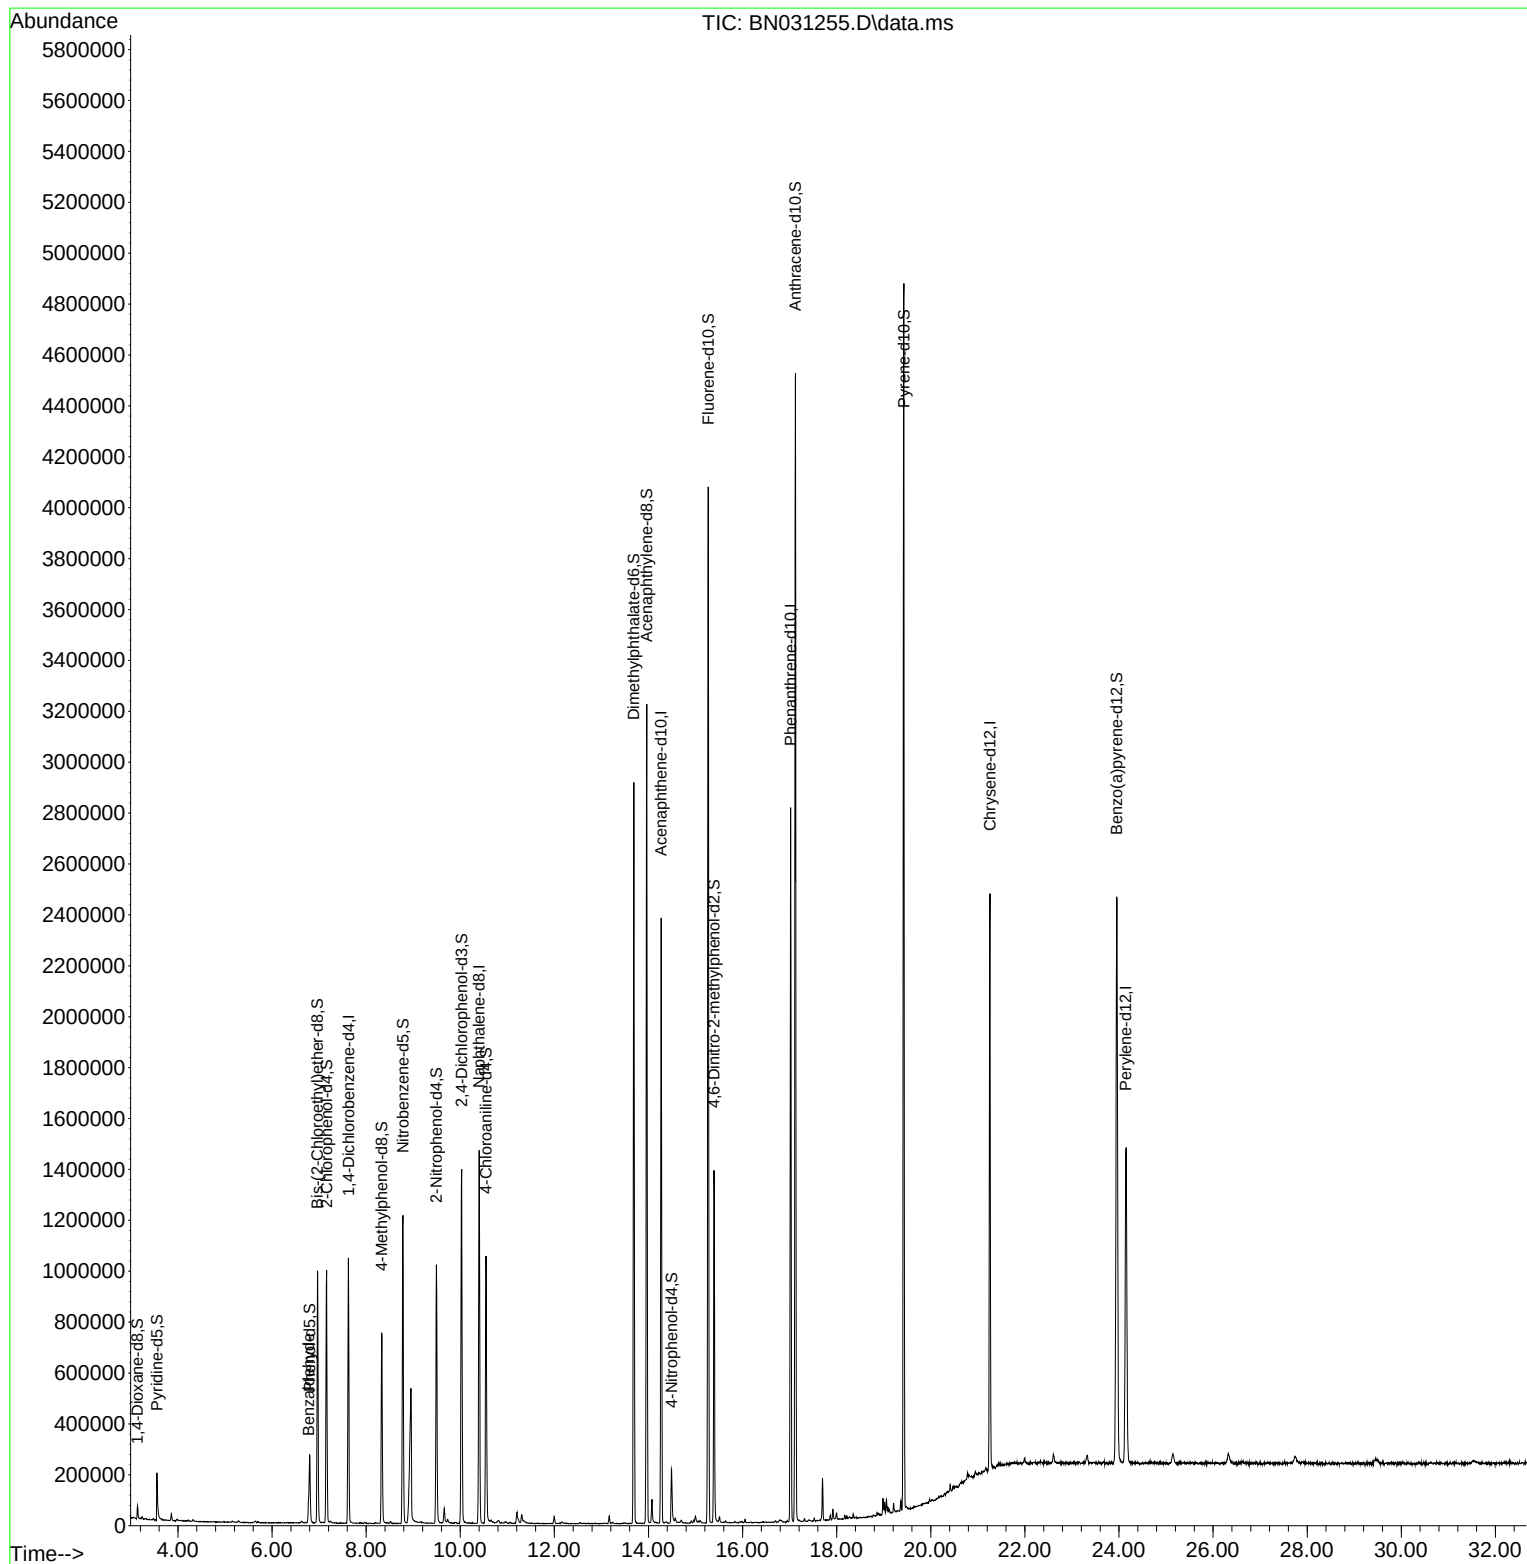

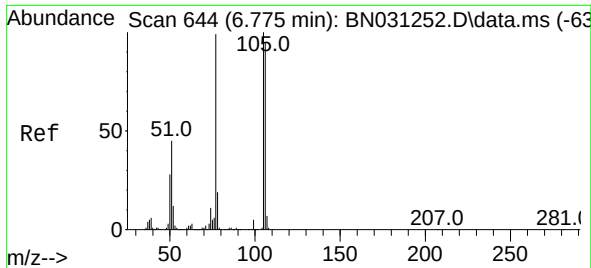

#6
Benzaldehyde
Concen: 2.554 ng/ul
RT: 6.775 min Scan# 644
Delta R.T. 0.000 min
Lab File: BN031255.D
Acq: 26 Apr 2024 22:23

Instrument :
BNA_N
ClientSampleId :
E08P1

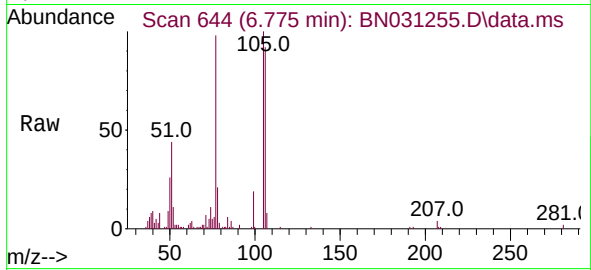

Tgt Ion:	77	Resp:	29488
Ion	Ratio	Lower	Upper
77	100		
105	101.7	80.0	120.0
106	93.3	75.0	112.6

