

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031239.D
 Acq On : 26 Apr 2024 10:32
 Operator : MA/JU
 Sample : PB160497BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK497

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rVB	88076	120632	1.46%	0.126%
2	3.540	91	94	119	rBV	1229051	2011616	24.27%	2.104%
3	3.858	144	148	153	rVB	16432	24033	0.29%	0.025%
4	6.793	640	647	664	rVB	1361599	2194040	26.47%	2.294%
5	6.963	669	676	690	rVB	1156995	1782391	21.50%	1.864%
6	7.152	700	708	725	rBV	1417659	2242528	27.05%	2.345%
7	7.616	780	787	795	rBV	1462683	2291555	27.64%	2.396%
8	8.328	900	908	925	rBV	1750396	2829275	34.13%	2.959%
9	8.775	975	984	995	rBV	1370649	2246434	27.10%	2.349%
10	9.493	1098	1106	1116	rBV	1183425	1928905	23.27%	2.017%
11	10.022	1189	1196	1211	rBV	1764858	2912344	35.13%	3.045%
12	10.398	1252	1260	1272	rBV	2165909	3535524	42.65%	3.697%
13	10.546	1277	1285	1300	rBV	1542978	2610386	31.49%	2.730%
14	11.993	1525	1531	1538	rBV	30323	51976	0.63%	0.054%
15	13.163	1723	1730	1736	rBV	25415	41877	0.51%	0.044%
16	13.687	1812	1819	1829	rBV	3313087	4695205	56.64%	4.910%
17	13.963	1858	1866	1882	rBV2	3651431	5554020	67.00%	5.808%
18	14.269	1911	1918	1928	rBV	3393014	4964724	59.89%	5.192%
19	14.375	1932	1936	1944	rVB8	5791	10271	0.12%	0.011%
20	14.486	1947	1955	1972	rBV	1630552	2449496	29.55%	2.561%
21	15.269	2080	2088	2100	rBV	4608062	6705342	80.89%	7.012%
22	15.398	2103	2110	2124	rBV	1662155	2363311	28.51%	2.471%
23	15.504	2124	2128	2134	rVB3	22252	36981	0.45%	0.039%
24	16.051	2216	2221	2226	rVB2	17626	26682	0.32%	0.028%
25	16.698	2327	2331	2335	rBV6	8618	12283	0.15%	0.013%
26	16.810	2346	2350	2355	rBV3	8583	11271	0.14%	0.012%
27	17.022	2379	2386	2396	rBV	4334493	6027938	72.72%	6.303%
28	17.122	2396	2403	2414	rBV	5043256	7282943	87.86%	7.616%
29	17.692	2496	2500	2505	rVB6	15506	19754	0.24%	0.021%
30	17.922	2535	2539	2543	rBV4	14357	20326	0.25%	0.021%
31	18.986	2715	2720	2725	rBV	71451	97507	1.18%	0.102%
32	19.057	2728	2732	2737	rVV	58762	77650	0.94%	0.081%
33	19.216	2755	2759	2761	rBV5	11721	15563	0.19%	0.016%
34	19.363	2781	2784	2788	rVB2	28095	28535	0.34%	0.030%
35	19.427	2788	2795	2802	rBV	6030707	8289422	100.00%	8.668%
36	20.416	2961	2963	2967	rVB3	28596	27493	0.33%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031239.D
Acq On : 26 Apr 2024 10:32
Operator : MA/JU
Sample : PB160497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M

Title : SVOA CALIBRATION

37	21.263	3101	3107	3116	rVB	4215356	6123404	73.87%	6.403%
38	23.962	3556	3566	3577	rBV2	3170783	7709292	93.00%	8.062%
39	24.162	3590	3600	3613	rVB2	2590454	6255525	75.46%	6.541%




Sum of corrected areas: 95628454

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031239.D
Acq On : 26 Apr 2024 10:32
Operator : MA/JU
Sample : PB160497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

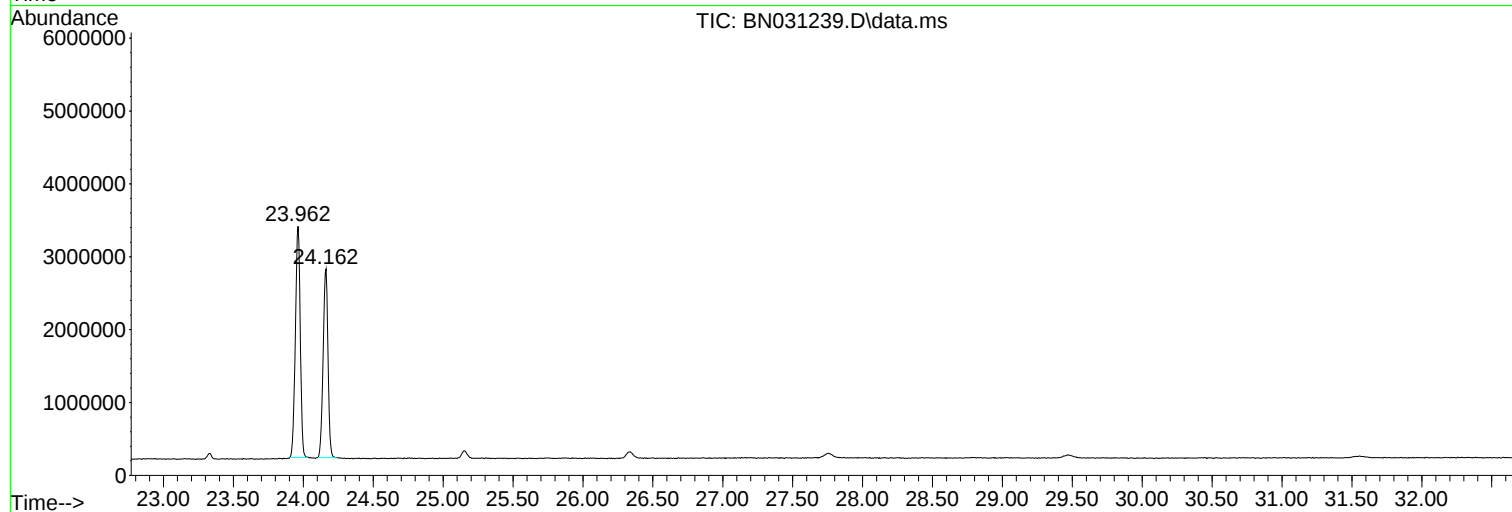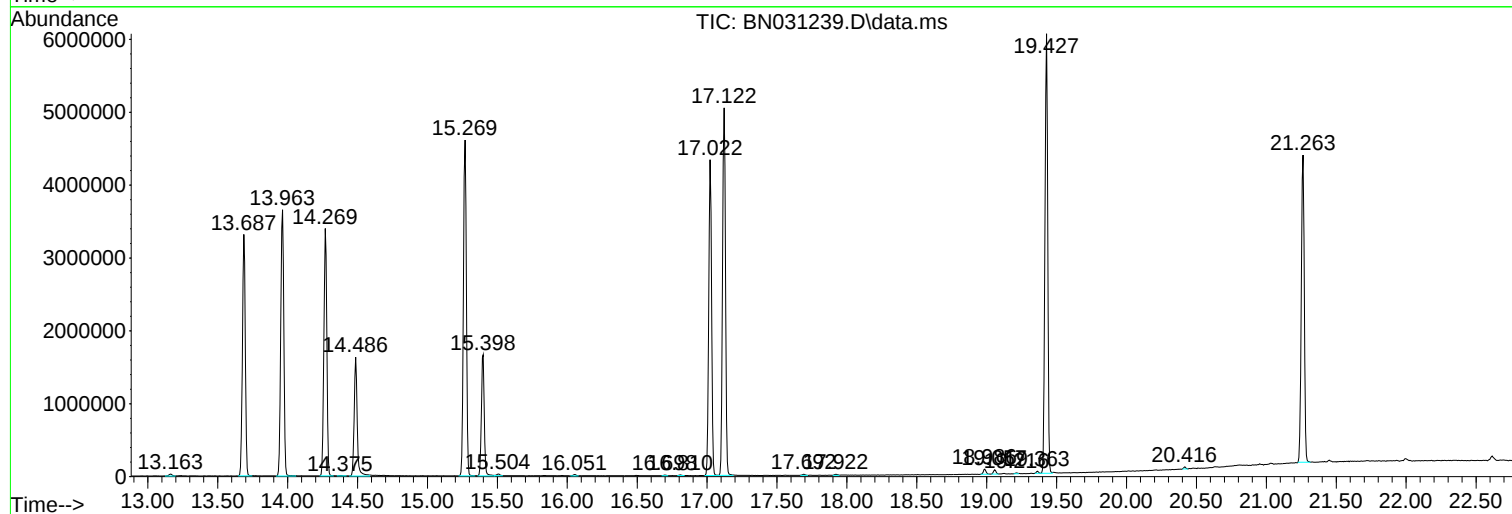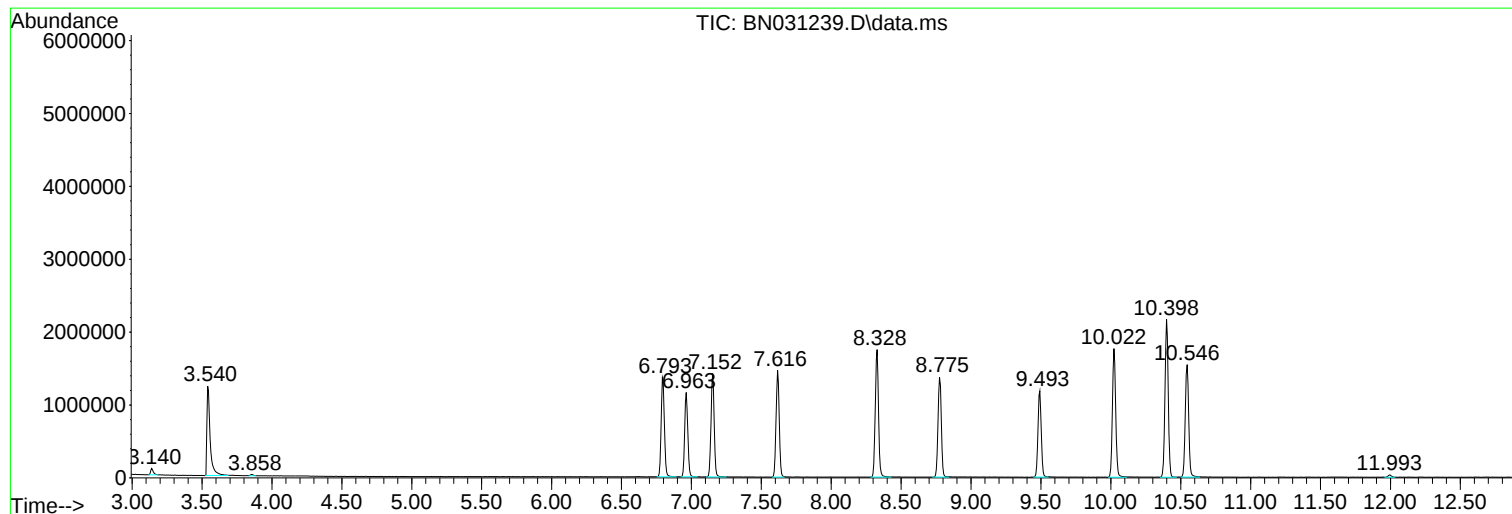

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031239.D
Acq On : 26 Apr 2024 10:32
Operator : MA/JU
Sample : PB160497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031239.D
Acq On : 26 Apr 2024 10:32
Operator : MA/JU
Sample : PB160497BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------