

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031253.D
Acq On : 26 Apr 2024 21:04
Operator : MA/JU
Sample : PB160561BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK561

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BN031253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	34	rVB	65582	88318	1.65%	0.138%
2	3.546	91	95	117	rBV	824662	1299906	24.34%	2.033%
3	3.858	145	148	155	rVB	15972	22329	0.42%	0.035%
4	6.799	642	648	662	rVB	1020353	1604033	30.04%	2.509%
5	6.964	670	676	687	rBV	839835	1322132	24.76%	2.068%
6	7.158	702	709	722	rBV	1078808	1691995	31.68%	2.646%
7	7.622	780	788	797	rBV	1054299	1633406	30.59%	2.555%
8	8.328	900	908	922	rBV	1278301	2068594	38.74%	3.236%
9	8.781	977	985	996	rBV	1004916	1652094	30.94%	2.584%
10	9.493	1099	1106	1121	rBV	892924	1417022	26.54%	2.216%
11	10.028	1189	1197	1213	rBV	1243940	2123095	39.76%	3.321%
12	10.399	1252	1260	1271	rBV	1468555	2515554	47.11%	3.935%
13	10.546	1273	1285	1300	rBV	1339812	2241919	41.98%	3.507%
14	11.999	1526	1532	1540	rVB2	22046	38192	0.72%	0.060%
15	13.163	1723	1730	1737	rBV2	24039	40396	0.76%	0.063%
16	13.240	1739	1743	1747	rVV4	3842	5927	0.11%	0.009%
17	13.687	1812	1819	1827	rBV	2414955	3327786	62.32%	5.205%
18	13.963	1857	1866	1873	rBV2	2645097	3982171	74.57%	6.229%
19	14.269	1911	1918	1928	rBV	2455282	3572214	66.89%	5.587%
20	14.381	1932	1937	1941	rVB6	3496	6009	0.11%	0.009%
21	14.487	1948	1955	1975	rBV	1062346	1617763	30.29%	2.530%
22	15.269	2080	2088	2095	rBV	3257209	4780088	89.51%	7.477%
23	15.393	2103	2109	2124	rBV	1144543	1516846	28.40%	2.373%
24	15.504	2124	2128	2134	rVB3	17000	27735	0.52%	0.043%
25	15.840	2180	2185	2187	rBV6	3474	5361	0.10%	0.008%
26	16.051	2216	2221	2228	rBV6	10000	17449	0.33%	0.027%
27	16.704	2328	2332	2336	rVB4	4917	7019	0.13%	0.011%
28	16.810	2345	2350	2355	rBV2	6797	11070	0.21%	0.017%
29	17.022	2379	2386	2393	rBV	2946396	4159825	77.90%	6.506%
30	17.122	2396	2403	2413	rVV	3473311	5035098	94.29%	7.875%
31	17.916	2534	2538	2543	rBV8	6169	12239	0.23%	0.019%
32	18.986	2715	2720	2725	rBV2	43496	61569	1.15%	0.096%
33	19.057	2728	2732	2736	rBV	36991	50365	0.94%	0.079%
34	19.363	2780	2784	2788	rBV4	19029	25060	0.47%	0.039%
35	19.422	2788	2794	2802	rBV	3919389	5340082	100.00%	8.352%
36	21.257	3100	3106	3113	rBV	2521936	3533851	66.18%	5.527%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031253.D
Acq On : 26 Apr 2024 21:04
Operator : MA/JU
Sample : PB160561BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK561

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	23.951	3556	3564	3579	rVB2	1695801	3936496	73.72%	6.157%
38	24.151	3589	3598	3610	rVB	1268954	3143217	58.86%	4.916%




Sum of corrected areas: 63934225

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031253.D
Acq On : 26 Apr 2024 21:04
Operator : MA/JU
Sample : PB160561BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

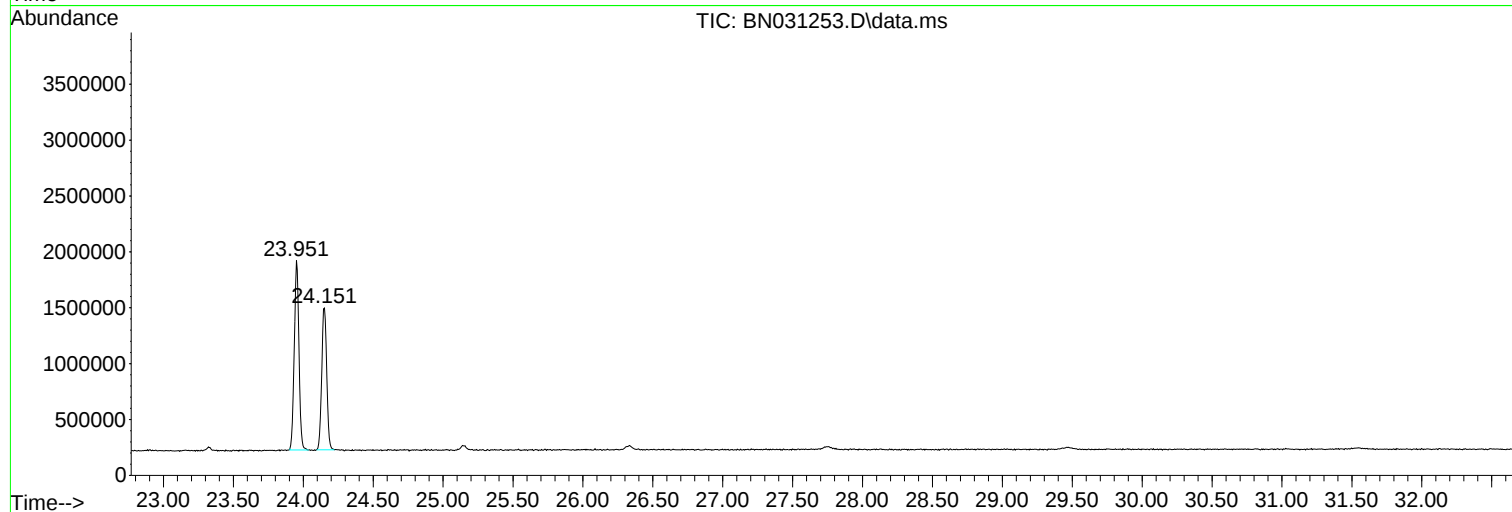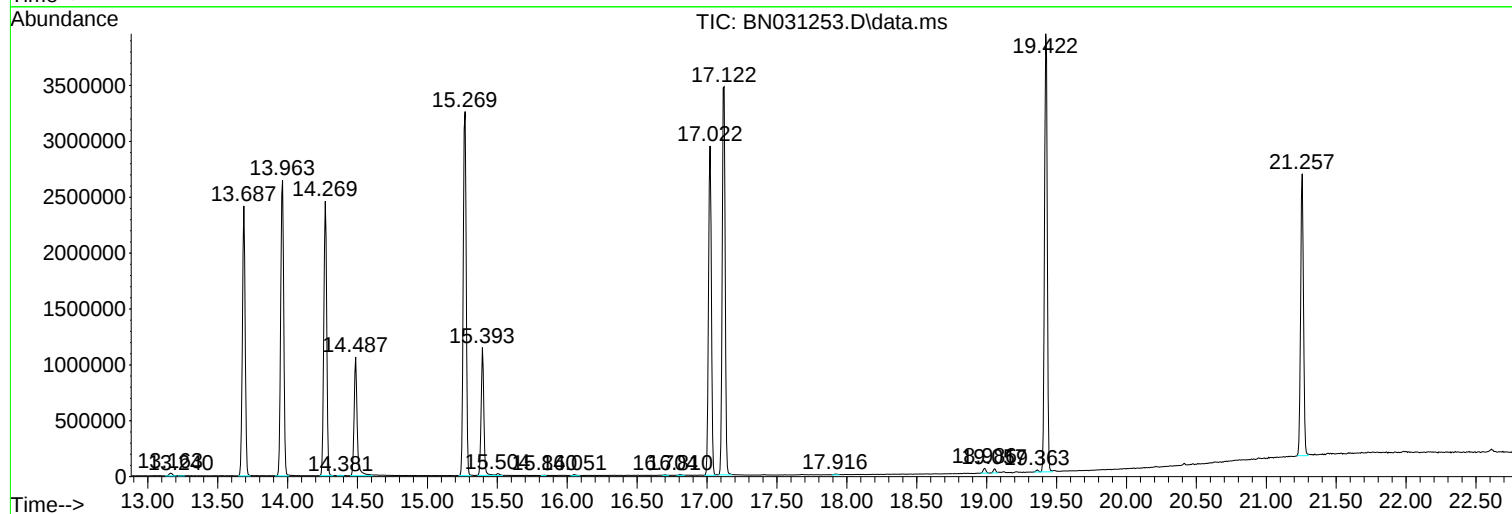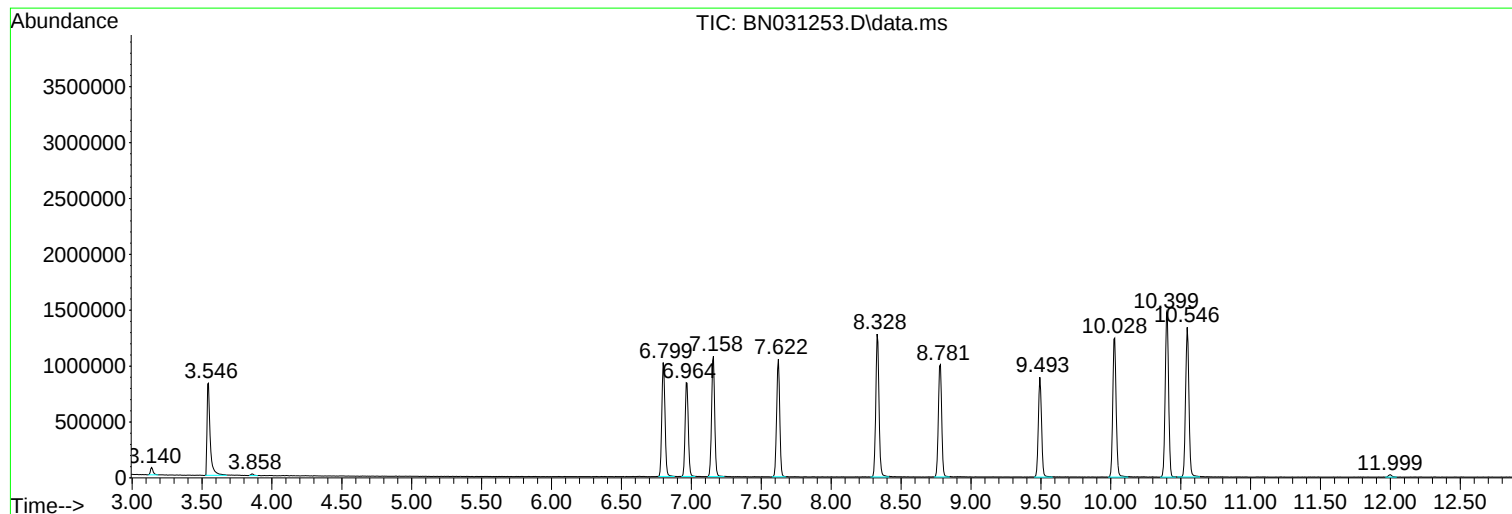

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031253.D
Acq On : 26 Apr 2024 21:04
Operator : MA/JU
Sample : PB160561BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031253.D
Acq On : 26 Apr 2024 21:04
Operator : MA/JU
Sample : PB160561BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------