

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031263.D
 Acq On : 27 Apr 2024 03:43
 Operator : MA/JU
 Sample : PB160384BL
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK384

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	21	26	36	rVB	62451	90561	1.46%	0.134%
2	3.540	91	94	112	rBV	865380	1309742	21.13%	1.939%
3	3.858	144	148	155	rVB	12549	19724	0.32%	0.029%
4	6.799	641	648	663	rBV	1099720	1705199	27.52%	2.524%
5	6.963	669	676	685	rBV	907201	1367414	22.07%	2.024%
6	7.151	699	708	720	rBV	1117395	1763749	28.46%	2.611%
7	7.616	781	787	796	rBV	934143	1484539	23.96%	2.197%
8	8.328	900	908	923	rBV	1386733	2214619	35.74%	3.278%
9	8.775	977	984	994	rBV	1057664	1711206	27.61%	2.533%
10	9.492	1098	1106	1115	rBV	914633	1463012	23.61%	2.165%
11	10.022	1189	1196	1213	rBV	1347448	2279901	36.79%	3.375%
12	10.398	1253	1260	1272	rVB	1442122	2348254	37.89%	3.476%
13	10.545	1277	1285	1301	rBV	1439347	2389577	38.56%	3.537%
14	11.992	1527	1531	1538	rBV2	20461	35964	0.58%	0.053%
15	13.163	1725	1730	1736	rBV	23571	39546	0.64%	0.059%
16	13.239	1738	1743	1748	rVB7	3380	6865	0.11%	0.010%
17	13.686	1812	1819	1829	rBV	2575360	3448698	55.65%	5.105%
18	13.957	1858	1865	1876	rBV	2727977	4182645	67.49%	6.191%
19	14.269	1911	1918	1925	rBV	2262611	3284618	53.00%	4.862%
20	14.486	1948	1955	1978	rBV	1098943	1695976	27.37%	2.510%
21	14.686	1985	1989	1993	rVB7	4235	7152	0.12%	0.011%
22	15.269	2081	2088	2095	rBV	3405141	5041684	81.36%	7.462%
23	15.392	2103	2109	2123	rBV	1083097	1451993	23.43%	2.149%
24	15.504	2124	2128	2133	rVB3	19115	29102	0.47%	0.043%
25	16.051	2215	2221	2225	rVB4	9215	13727	0.22%	0.020%
26	16.804	2347	2349	2354	rVB4	7370	10073	0.16%	0.015%
27	17.022	2379	2386	2396	rBV	2662642	3884156	62.68%	5.749%
28	17.122	2396	2403	2418	rVV2	3784882	5477017	88.38%	8.107%
29	18.274	2594	2599	2602	rBV6	4525	8823	0.14%	0.013%
30	18.986	2715	2720	2725	rBV3	49446	72701	1.17%	0.108%
31	19.051	2727	2731	2736	rBV	41223	58312	0.94%	0.086%
32	19.363	2781	2784	2787	rBV	18484	20921	0.34%	0.031%
33	19.421	2788	2794	2802	rBV	4526461	6197120	100.00%	9.173%
34	21.257	3100	3106	3115	rBV2	2686092	3867704	62.41%	5.725%
35	23.951	3555	3564	3577	rVB	2094758	5026082	81.10%	7.439%
36	24.151	3589	3598	3613	rVB	1488814	3552787	57.33%	5.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031263.D
Acq On : 27 Apr 2024 03:43
Operator : MA/JU
Sample : PB160384BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK384

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 67561163

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031263.D
Acq On : 27 Apr 2024 03:43
Operator : MA/JU
Sample : PB160384BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK384

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

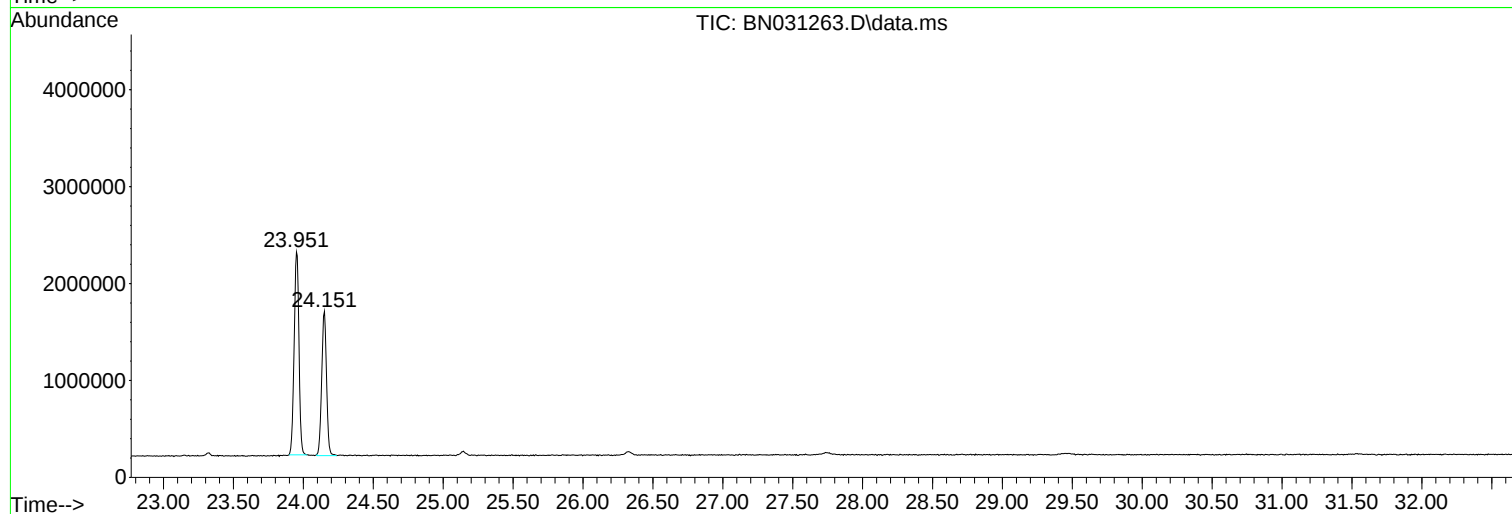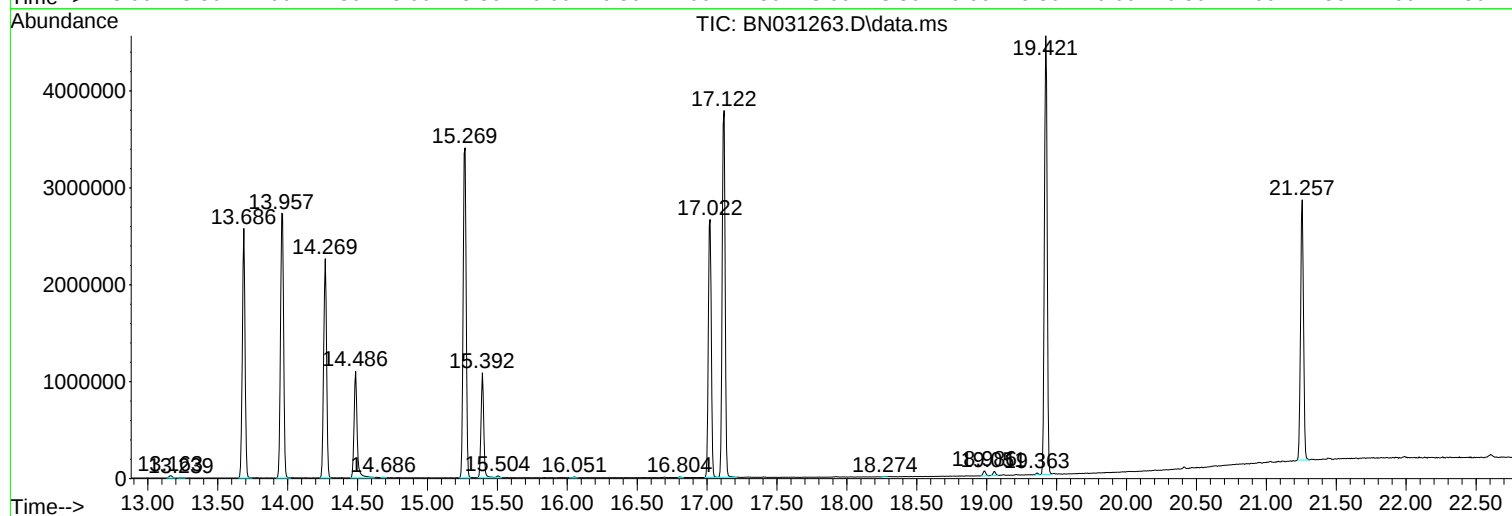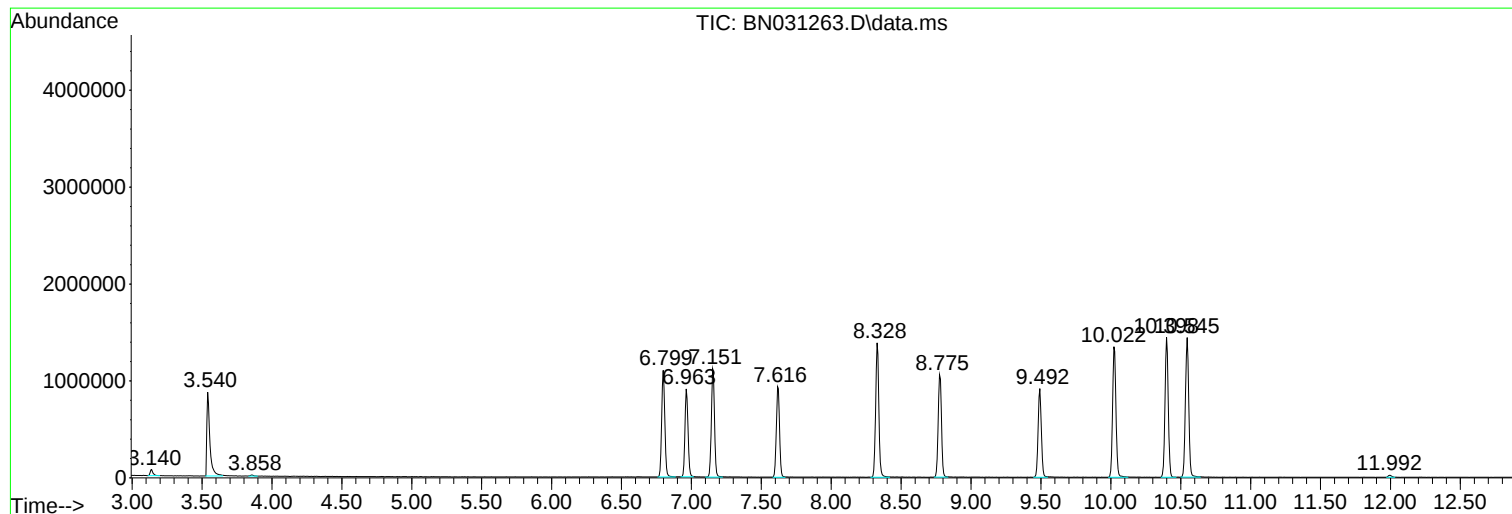

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031263.D
Acq On : 27 Apr 2024 03:43
Operator : MA/JU
Sample : PB160384BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK384

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031263.D
Acq On : 27 Apr 2024 03:43
Operator : MA/JU
Sample : PB160384BL
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK384

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------