

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
 Data File : BN031264.D
 Acq On : 27 Apr 2024 04:22
 Operator : MA/JU
 Sample : PB160415BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK415

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.140	22	26	32	rBV	79417	103574	1.60%	0.135%
2	3.540	91	94	113	rBV	1171546	1714259	26.48%	2.228%
3	3.858	144	148	156	rVB2	14413	22213	0.34%	0.029%
4	6.799	641	648	660	rBV	1291288	1981085	30.60%	2.575%
5	6.963	669	676	688	rBV	1034483	1582578	24.44%	2.057%
6	7.152	701	708	719	rBV	1259881	1993702	30.79%	2.591%
7	7.622	779	788	800	rBV	1258687	2045592	31.59%	2.659%
8	8.328	901	908	922	rBV	1610096	2559938	39.54%	3.327%
9	8.775	977	984	997	rBV	1210603	1965714	30.36%	2.555%
10	9.493	1099	1106	1117	rBV	1057584	1703080	26.30%	2.214%
11	10.022	1189	1196	1208	rBV	1573350	2641510	40.80%	3.433%
12	10.399	1252	1260	1272	rBV	1920899	3169234	48.95%	4.119%
13	10.546	1276	1285	1300	rBV	1404001	2345572	36.23%	3.049%
14	11.993	1525	1531	1537	rBV2	25756	44921	0.69%	0.058%
15	13.163	1724	1730	1736	rBV	22153	34899	0.54%	0.045%
16	13.228	1736	1741	1746	rVB5	4159	6500	0.10%	0.008%
17	13.687	1812	1819	1828	rBV	2769113	3873122	59.82%	5.034%
18	13.957	1858	1865	1879	rBV	3111271	4756215	73.46%	6.182%
19	14.269	1910	1918	1926	rBV	3021429	4293016	66.30%	5.580%
20	14.375	1933	1936	1942	rVB6	4029	8271	0.13%	0.011%
21	14.487	1948	1955	1976	rBV	1202089	1885155	29.12%	2.450%
22	15.269	2080	2088	2100	rVB	3803893	5676307	87.67%	7.378%
23	15.392	2102	2109	2123	rVV	1265928	1730209	26.72%	2.249%
24	15.504	2123	2128	2133	rVB2	19283	31287	0.48%	0.041%
25	16.051	2217	2221	2227	rVB4	15173	19404	0.30%	0.025%
26	16.698	2328	2331	2335	rVB5	6309	8904	0.14%	0.012%
27	16.810	2344	2350	2355	rVB3	7081	11700	0.18%	0.015%
28	17.022	2379	2386	2396	rBV	3467066	4952490	76.49%	6.437%
29	17.116	2396	2402	2417	rVB	4131195	5964063	92.11%	7.752%
30	17.692	2496	2500	2506	rVB7	14219	18356	0.28%	0.024%
31	17.916	2534	2538	2542	rBV6	12494	16118	0.25%	0.021%
32	18.980	2715	2719	2726	rVB	52530	73224	1.13%	0.095%
33	19.057	2727	2732	2736	rBV	45392	60678	0.94%	0.079%
34	19.210	2754	2758	2763	rBV7	12629	22123	0.34%	0.029%
35	19.357	2780	2783	2788	rBV	27991	34833	0.54%	0.045%
36	19.422	2788	2794	2802	rBV	4689530	6474738	100.00%	8.416%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031264.D
Acq On : 27 Apr 2024 04:22
Operator : MA/JU
Sample : PB160415BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK415

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Title : SVOA CALIBRATION

37	20.416	2960	2963	2967	rBV3	22542	26494	0.41%	0.034%
38	21.257	3100	3106	3116	rBV	2924790	4262610	65.83%	5.540%
39	23.951	3555	3564	3577	rVB2	2080503	4852356	74.94%	6.307%
40	24.151	3589	3598	3610	rVB	1656628	3969801	61.31%	5.160%




Sum of corrected areas: 76935845

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031264.D
Acq On : 27 Apr 2024 04:22
Operator : MA/JU
Sample : PB160415BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

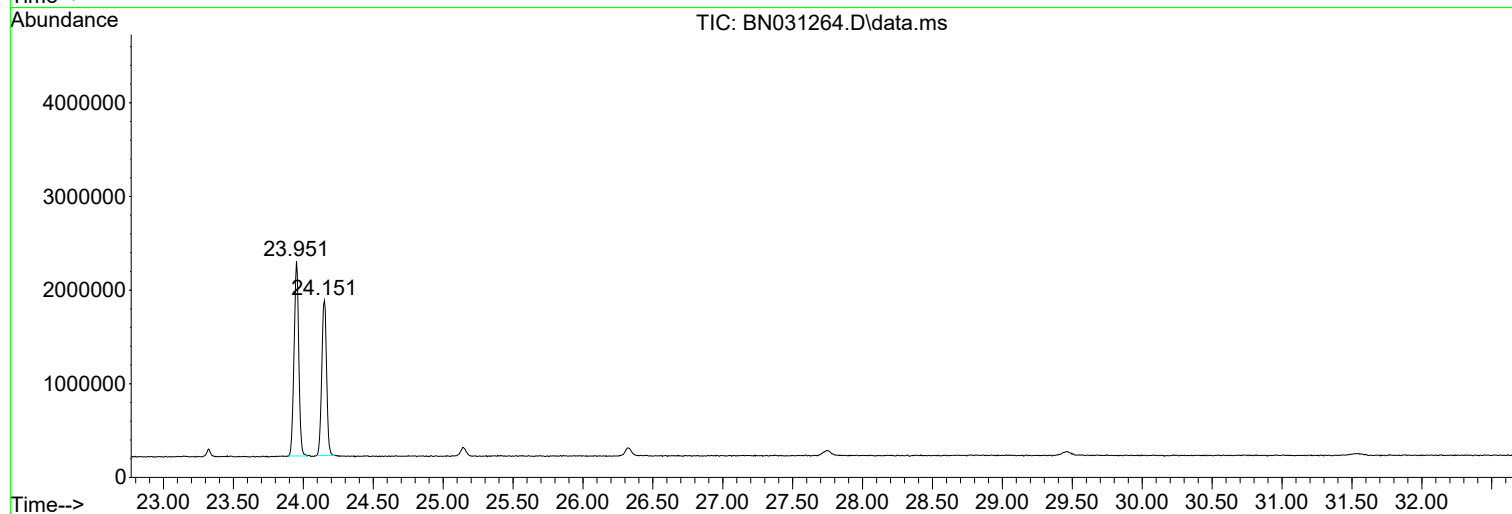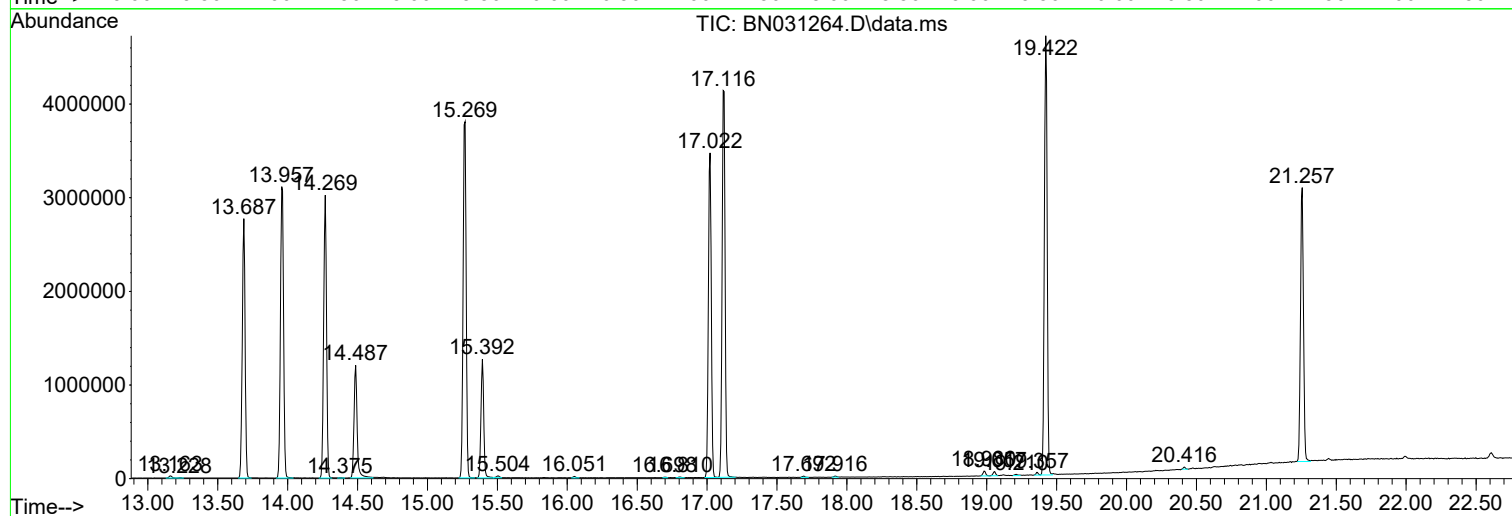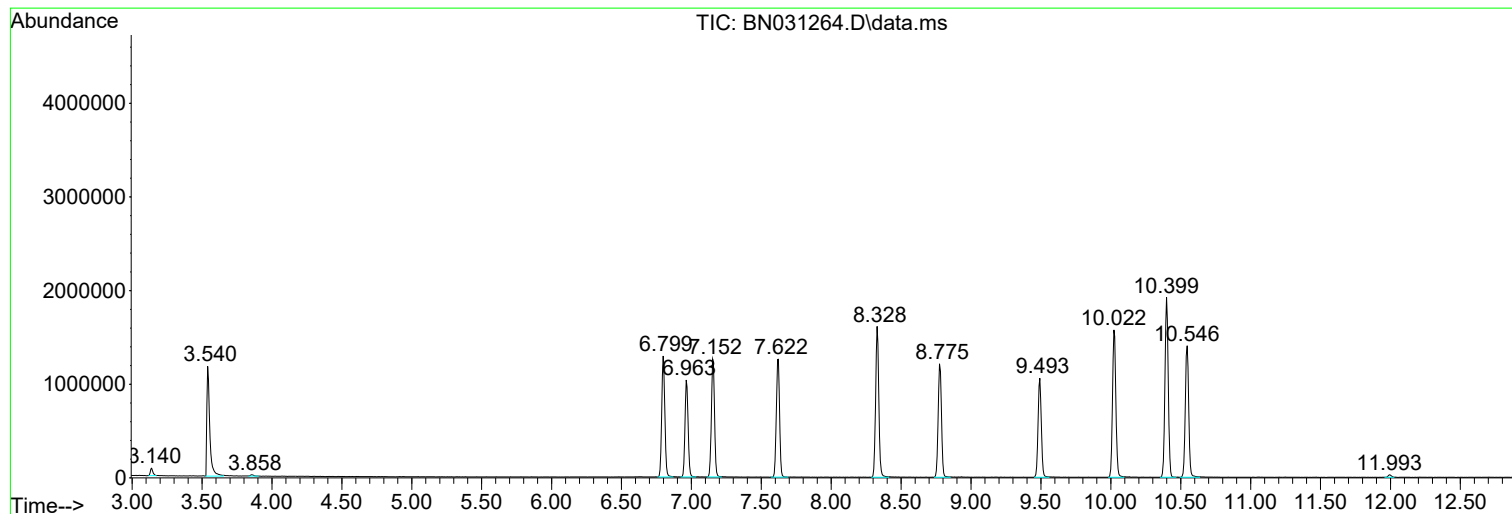

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031264.D
Acq On : 27 Apr 2024 04:22
Operator : MA/JU
Sample : PB160415BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042624\
Data File : BN031264.D
Acq On : 27 Apr 2024 04:22
Operator : MA/JU
Sample : PB160415BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK415

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN041924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------