
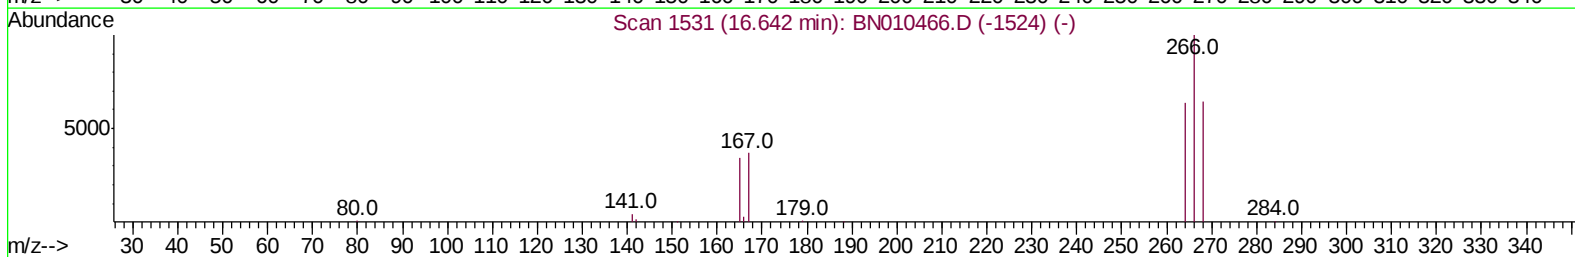
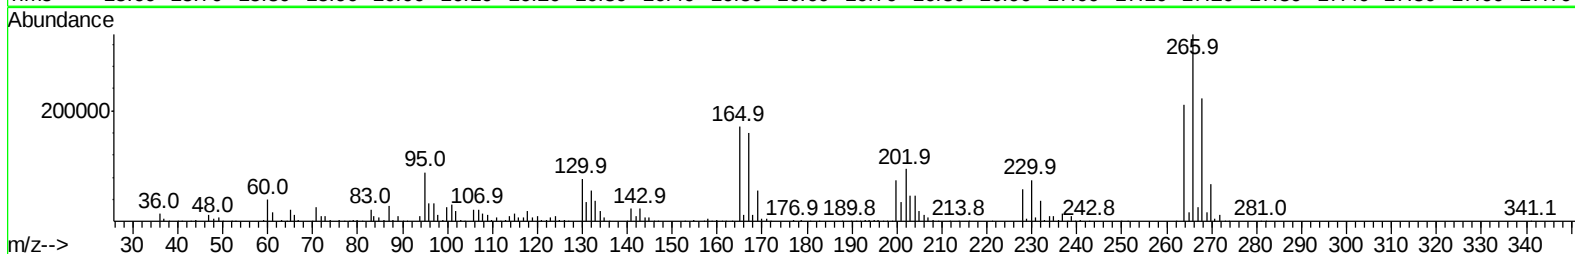


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN042820\
 Data File : BN010632.D
 Acq On : 28 Apr 2020 20:36
 Operator : CG/JU
 Sample : DFTPP71
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 21:11:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 28 11:13:37 2020
 Response via : Initial Calibration

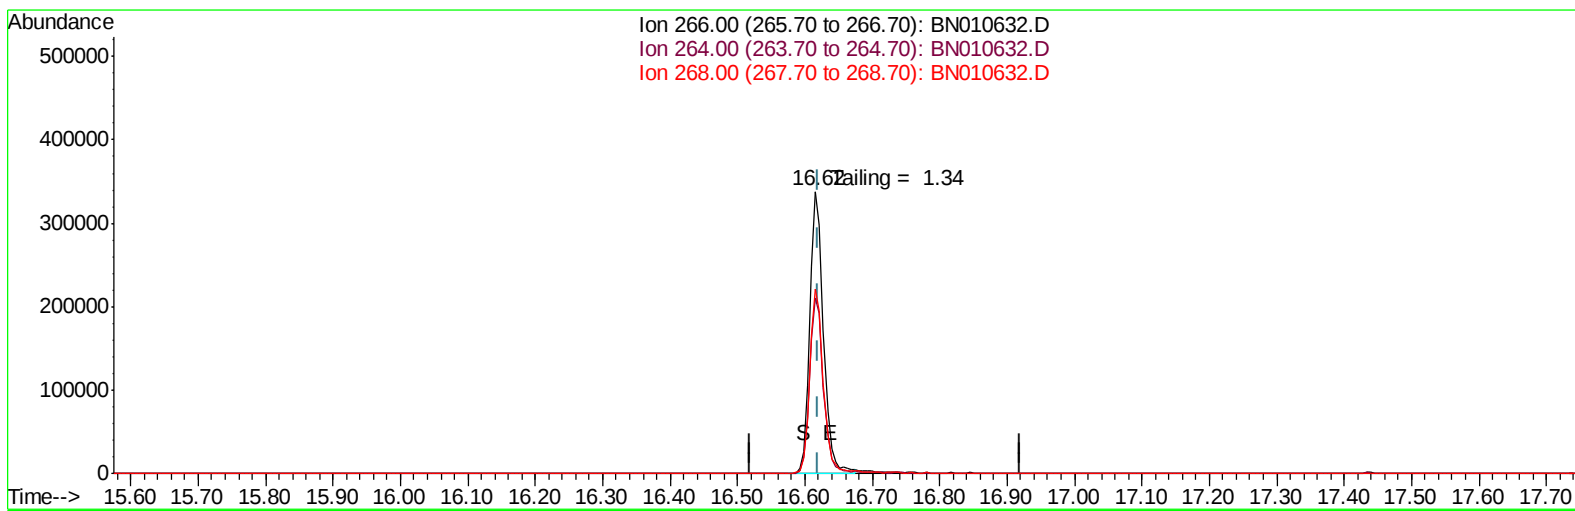

TIC: BN010632.D

(22) Pentachlorophenol

16.616min (-0.004) 0.00ng

response 480264

Ion	Exp%	Act%
266.00	100	100
264.00	64.70	62.19
268.00	67.10	65.57
0.00	0.00	0.00