


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042820\
 Data File : BN010617.D
 Acq On : 28 Apr 2020 08:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 28 11:13:37 2020

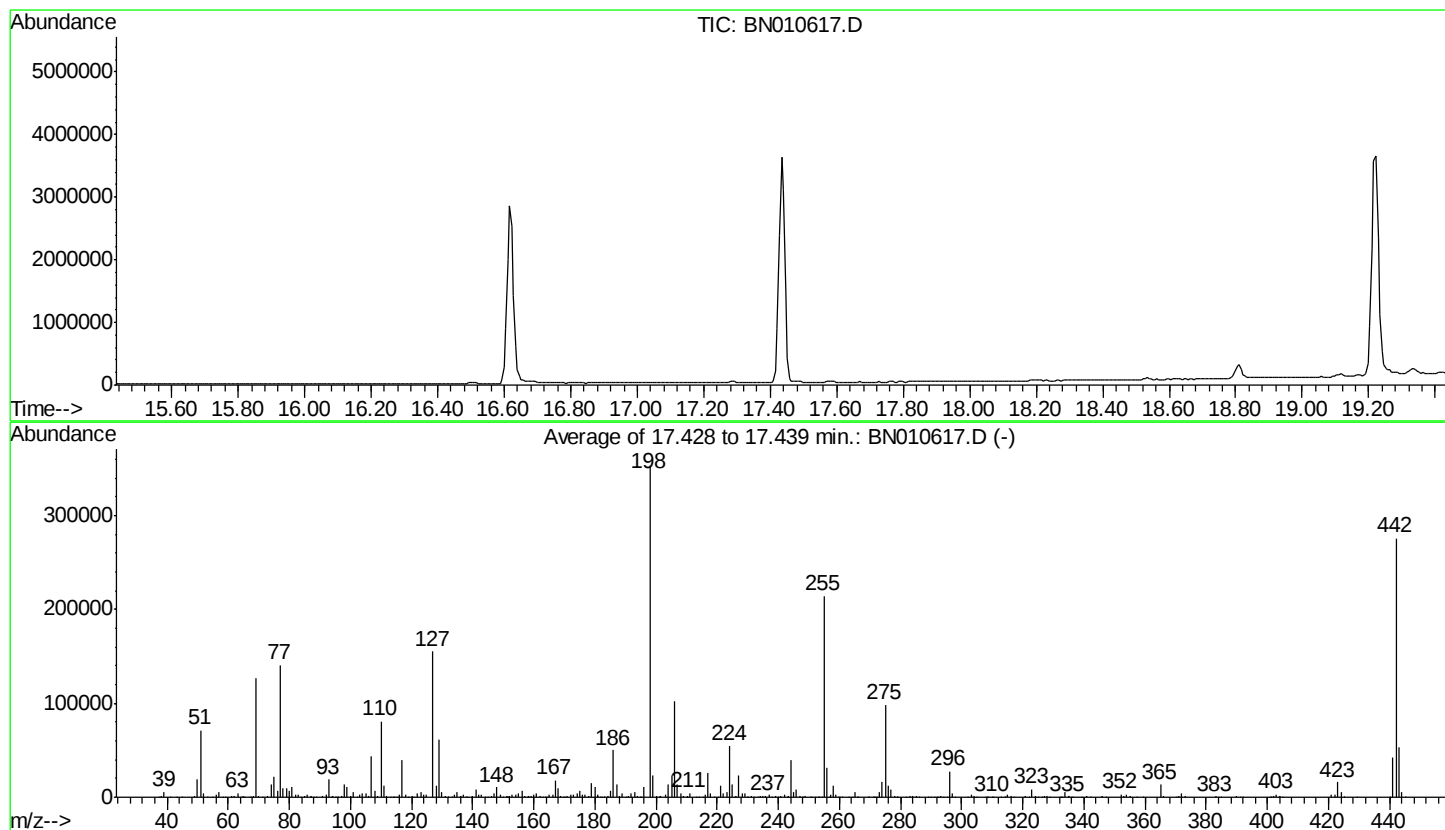

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.1	71133	PASS
68	69	0.00	2	0.9	1104	PASS
69	198	0.00	100	35.7	126194	PASS
70	69	0.00	2	0.8	1031	PASS
127	198	10	80	43.9	155136	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	353066	PASS
199	198	5	9	6.7	23794	PASS
275	198	10	60	27.9	98594	PASS
365	198	1	100	3.8	13243	PASS
441	198	0.01	100	12.1	42712	PASS
442	198	50	100	78.2	275925	PASS
443	442	15	24	19.3	53154	PASS