


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042820\
 Data File : BN010632.D
 Acq On : 28 Apr 2020 20:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 28 11:13:37 2020

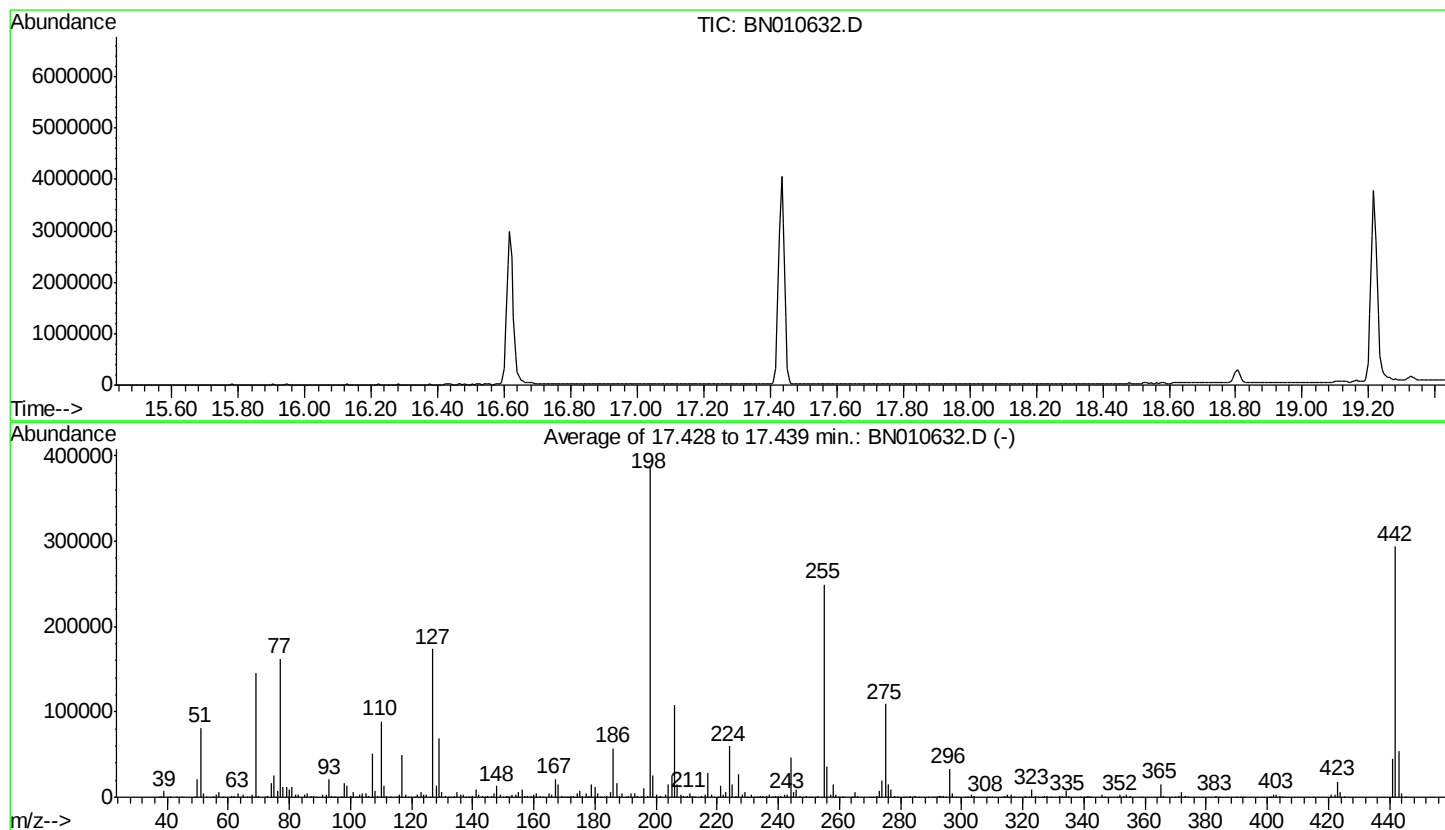

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	81728	PASS
68	69	0.00	2	2.0	2914	PASS
69	198	0.00	100	37.4	145205	PASS
70	69	0.00	2	0.6	863	PASS
127	198	10	80	44.8	173952	PASS
197	198	0.00	2	0.2	880	PASS
198	198	100	100	100.0	388501	PASS
199	198	5	9	6.6	25712	PASS
275	198	10	60	28.0	108928	PASS
365	198	1	100	4.0	15529	PASS
441	198	0.01	100	11.7	45266	PASS
442	198	50	100	75.6	293674	PASS
443	442	15	24	18.3	53874	PASS