

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN042919\
 Data File : BN005352.D
 Acq On : 29 Apr 2019 10:35
 Operator : JU/SJ
 Sample : PB119190BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB119190BL

Quant Time: Apr 30 01:07:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	399194	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1744334	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1042183	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2395964	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	1953466	20.00	ng/ul	0.00
85) Perylene-d12	23.45	264	1911402	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	71827	8.69	ng/uL	0.00
5) Phenol-d5	6.77	99	1376676	43.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	797997	40.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	1105714	46.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	1109852	45.28	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	570340	53.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	639332	58.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	1143361	45.83	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.49	131	1568824	60.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	3346408	44.23	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	4359932	46.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	562660	47.10	ng/ul	0.00
57) Fluorene-d10	15.23	176	2984513	47.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	439071	40.74	ng/ul	0.00
70) Anthracene-d10	17.08	188	4636899	46.17	ng/ul	0.00
78) Pyrene-d10	19.40	212	4813164	48.16	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.31	264	3966042	47.48	ng/ul	0.00

Target Compounds


					Ovalue
83) Bis(2-ethylhexyl)phthalate	21.16	149	250091	3.262 ng/ul	98
86) Di-n-octyl phthalate	22.06	149	253563	2.166 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042919\
Data File : BN005352.D
Acq On : 29 Apr 2019 10:35
Operator : JU/SJ
Sample : PB119190BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB119190BL

Quant Time: Apr 30 01:07:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

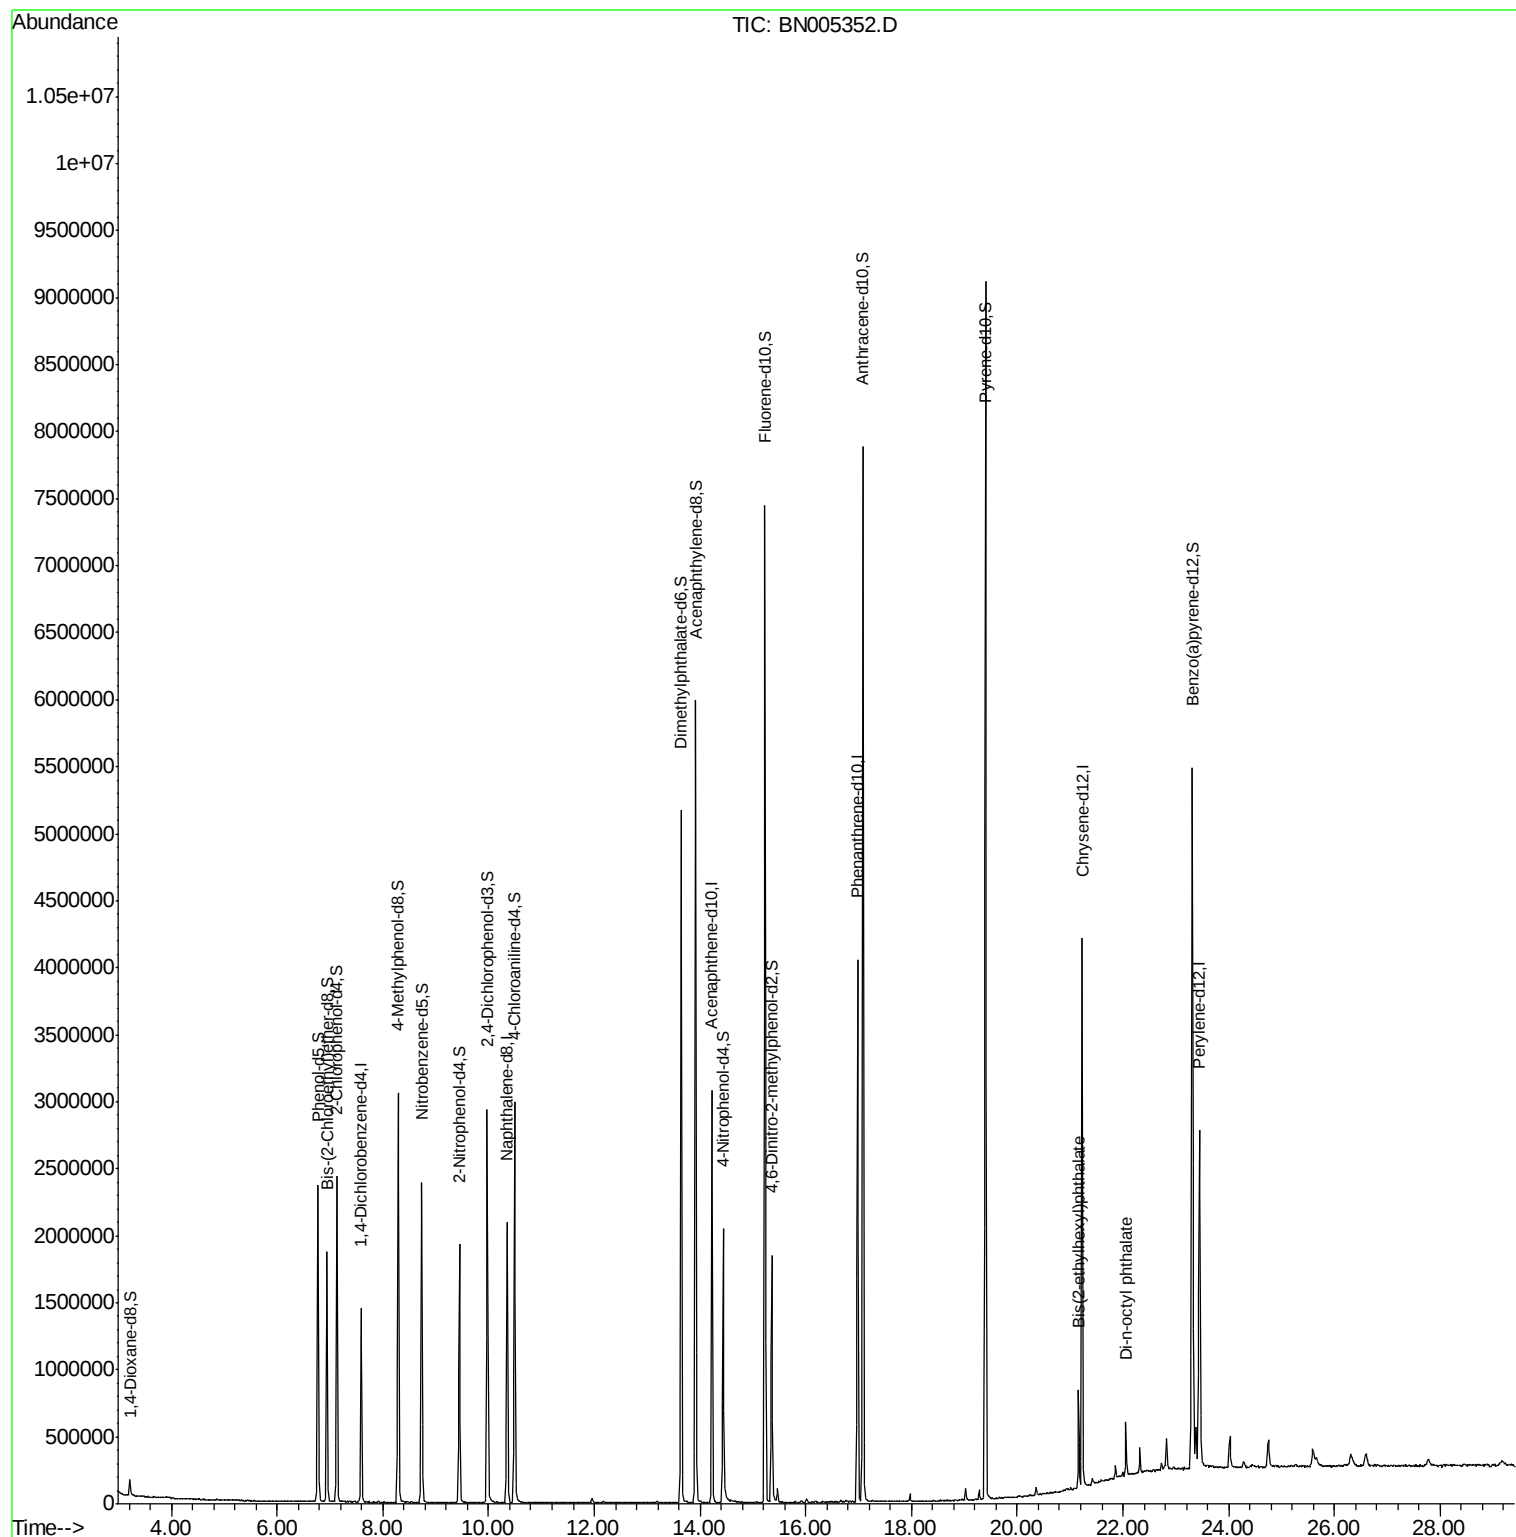


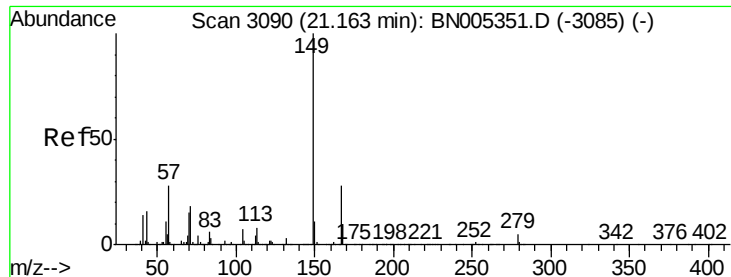




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 3.262 ng/ul
 RT: 21.16 min Scan# 3090
 Delta R.T. -0.01 min
 Lab File: BN005352.D
 Acq: 29 Apr 2019 10:35

Instrument :
 BNA_N
 ClientSampleId :
 PB119190BL

Tot Ion:149 Resp: 250091
 Ion Ratio Lower Upper
 149 100
 167 29.2 22.3 33.5
 279 4.2 3.3 4.9

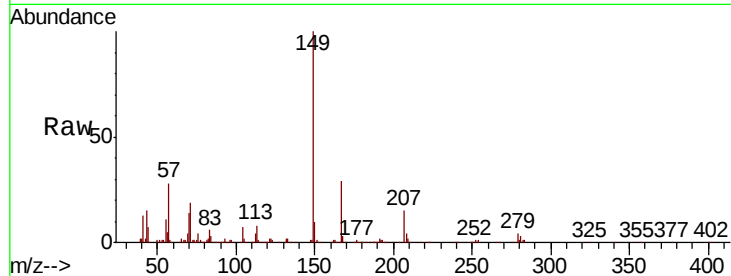


Abundance Ion 149.00 (148.70 to 149.70): E
 300000
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

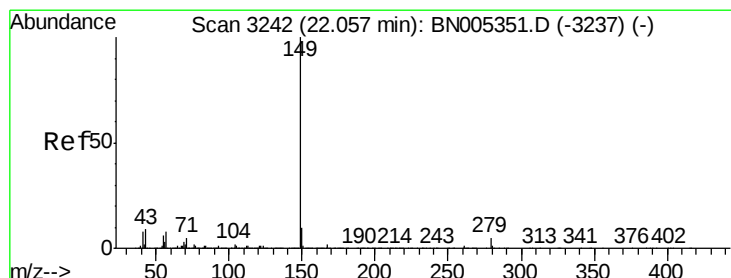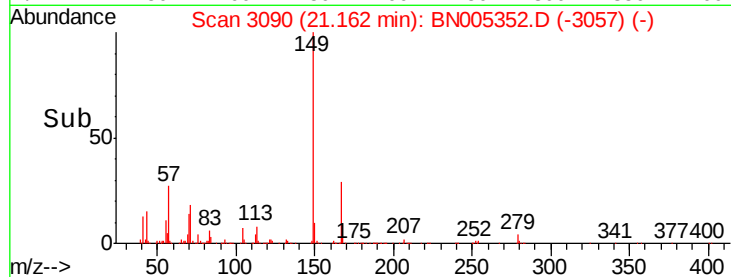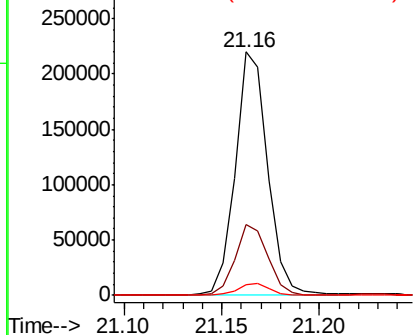

#86
 Di-n-octyl phthalate
 Concen: 2.166 ng/ul
 RT: 22.06 min Scan# 3242
 Delta R.T. 0.00 min
 Lab File: BN005352.D
 Acq: 29 Apr 2019 10:35

Tgt Ion:149 Resp: 253563

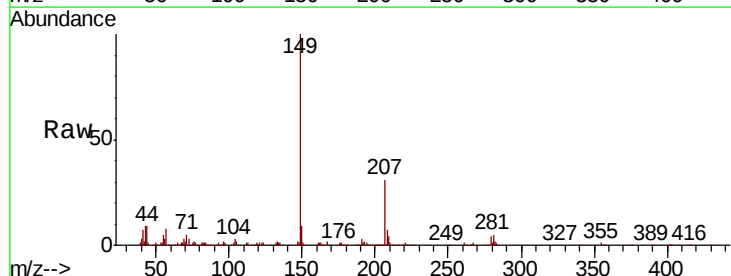

Abundance Ion 149.00 (148.70 to 149.70): E

