

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042919\
 Data File : BN005353.D
 Acq On : 29 Apr 2019 11:43
 Operator : JU/SJ
 Sample : K2470-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5135

Quant Time: Apr 30 00:52:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	377417	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1618371	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	972341	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2196619	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	1642968	20.00	ng/ul	-0.01
85) Perylene-d12	23.43	264	1634288	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	40354	5.16	ng/uL	0.00
5) Phenol-d5	6.78	99	879647	29.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	523660	28.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	710556	31.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	714065	30.82	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	365396	36.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	410947	40.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	737221	31.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	1012944	42.43	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	2256690	31.97	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2882977	33.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	340768	30.58	ng/ul	0.00
57) Fluorene-d10	15.23	176	2000677	33.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	269556	27.28	ng/ul	0.00
70) Anthracene-d10	17.08	188	3061027	33.24	ng/ul	0.00
78) Pyrene-d10	19.39	212	3122835	37.16	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	2405492	33.68	ng/ul	-0.01


Target Compounds					Ovalue
44) Dimethylphthalate	13.69	163	484404	6.887	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042919\
Data File : BN005353.D
Acq On : 29 Apr 2019 11:43
Operator : JU/SJ
Sample : K2470-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
A5135

Quant Time: Apr 30 00:52:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

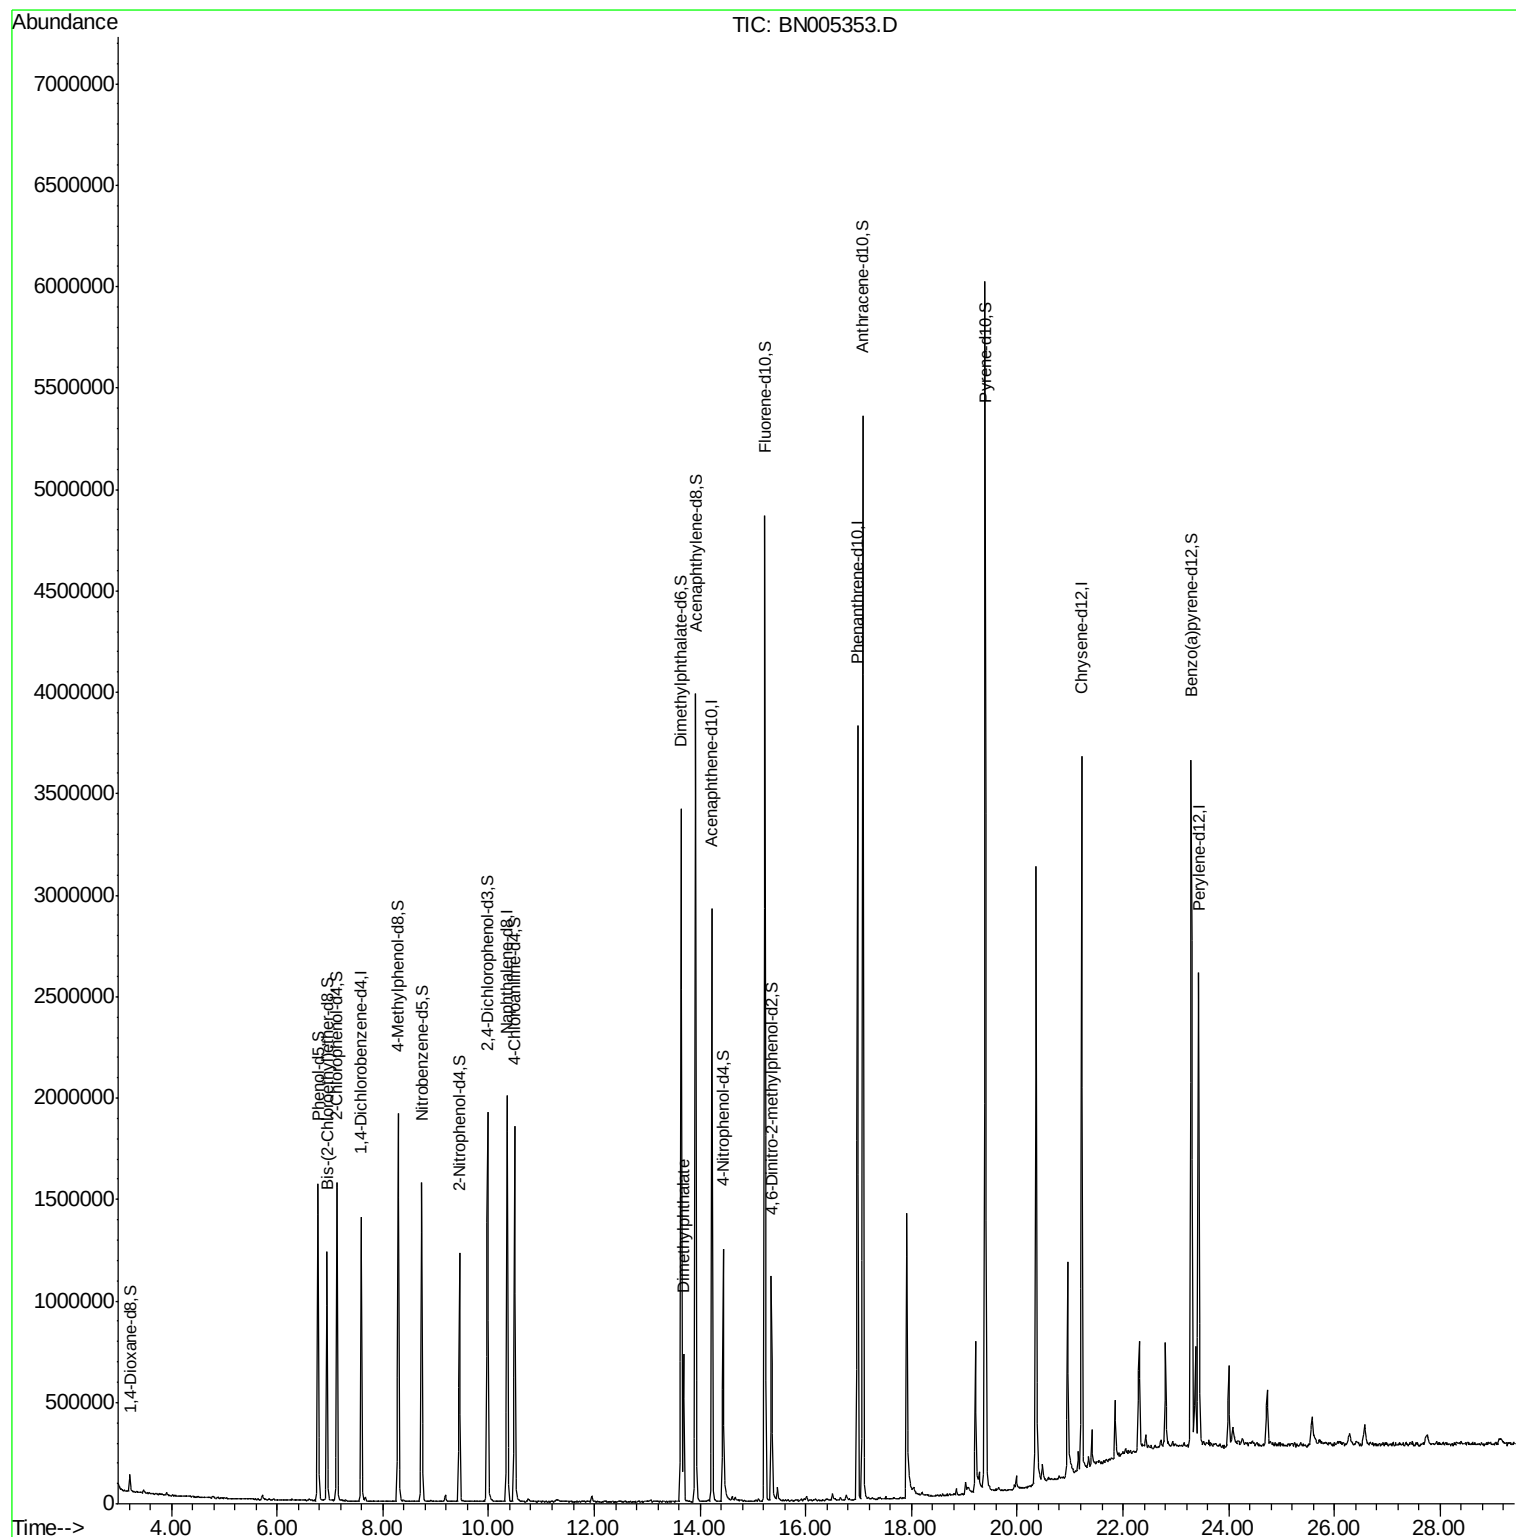

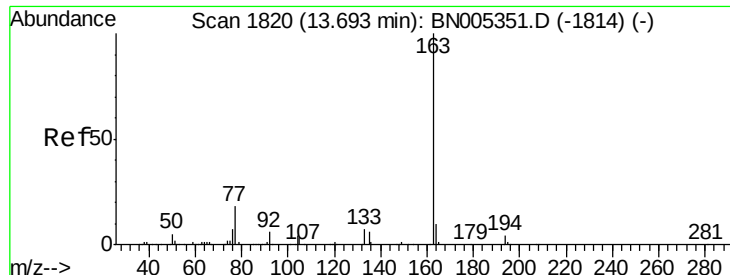

#44

Dimethylphthalate

Concen: 6.887 ng/ul

RT: 13.69 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BN005353.D

Acq: 29 Apr 2019 11:43

Instrument :

BNA_N

ClientSampleId :

A5135


Tot Ion:163 Resp: 484404

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 9.7 8.1 12.1

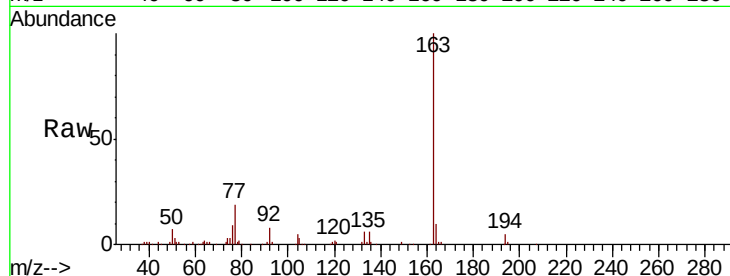

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

