

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042920\
 Data File : BN010661.D
 Acq On : 29 Apr 2020 18:55
 Operator : CG/JU
 Sample : L2392-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF7

Quant Time: Apr 30 03:54:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 30 02:18:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	414357	20.00	ng/ul	0.00
18) Naphthalene-d8	10.33	136	1834322	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	1159178	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	2589888	20.00	ng/ul	0.00
78) Chrysene-d12	21.16	240	2134300	20.00	ng/ul	-0.01
86) Perylene-d12	23.33	264	1995922	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	34239	4.32	ng/uL	0.00
5) Phenol-d5	6.77	99	842088	25.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	452598	27.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.12	132	699241	25.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	728896	26.42	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	359319	25.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	398693	25.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	765600	24.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	1001524	28.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.63	166	2409592	28.02	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	2925608	27.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.42	143	318329	19.01	ng/ul	0.00
58) Fluorene-d10	15.20	176	2170945	28.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.33	200	231139	17.08	ng/ul	0.00
71) Anthracene-d10	17.05	188	3371932	28.11	ng/ul	0.00
79) Pyrene-d10	19.36	212	3654946	30.34	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2863554	27.66	ng/ul	-0.02


Target Compounds						Qvalue
45) Dimethylphthalate	13.67	163	722657	8.09	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN042920\
Data File : BN010661.D
Acq On : 29 Apr 2020 18:55
Operator : CG/JU
Sample : L2392-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AF7

Quant Time: Apr 30 03:54:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 30 02:18:10 2020
Response via : Initial Calibration

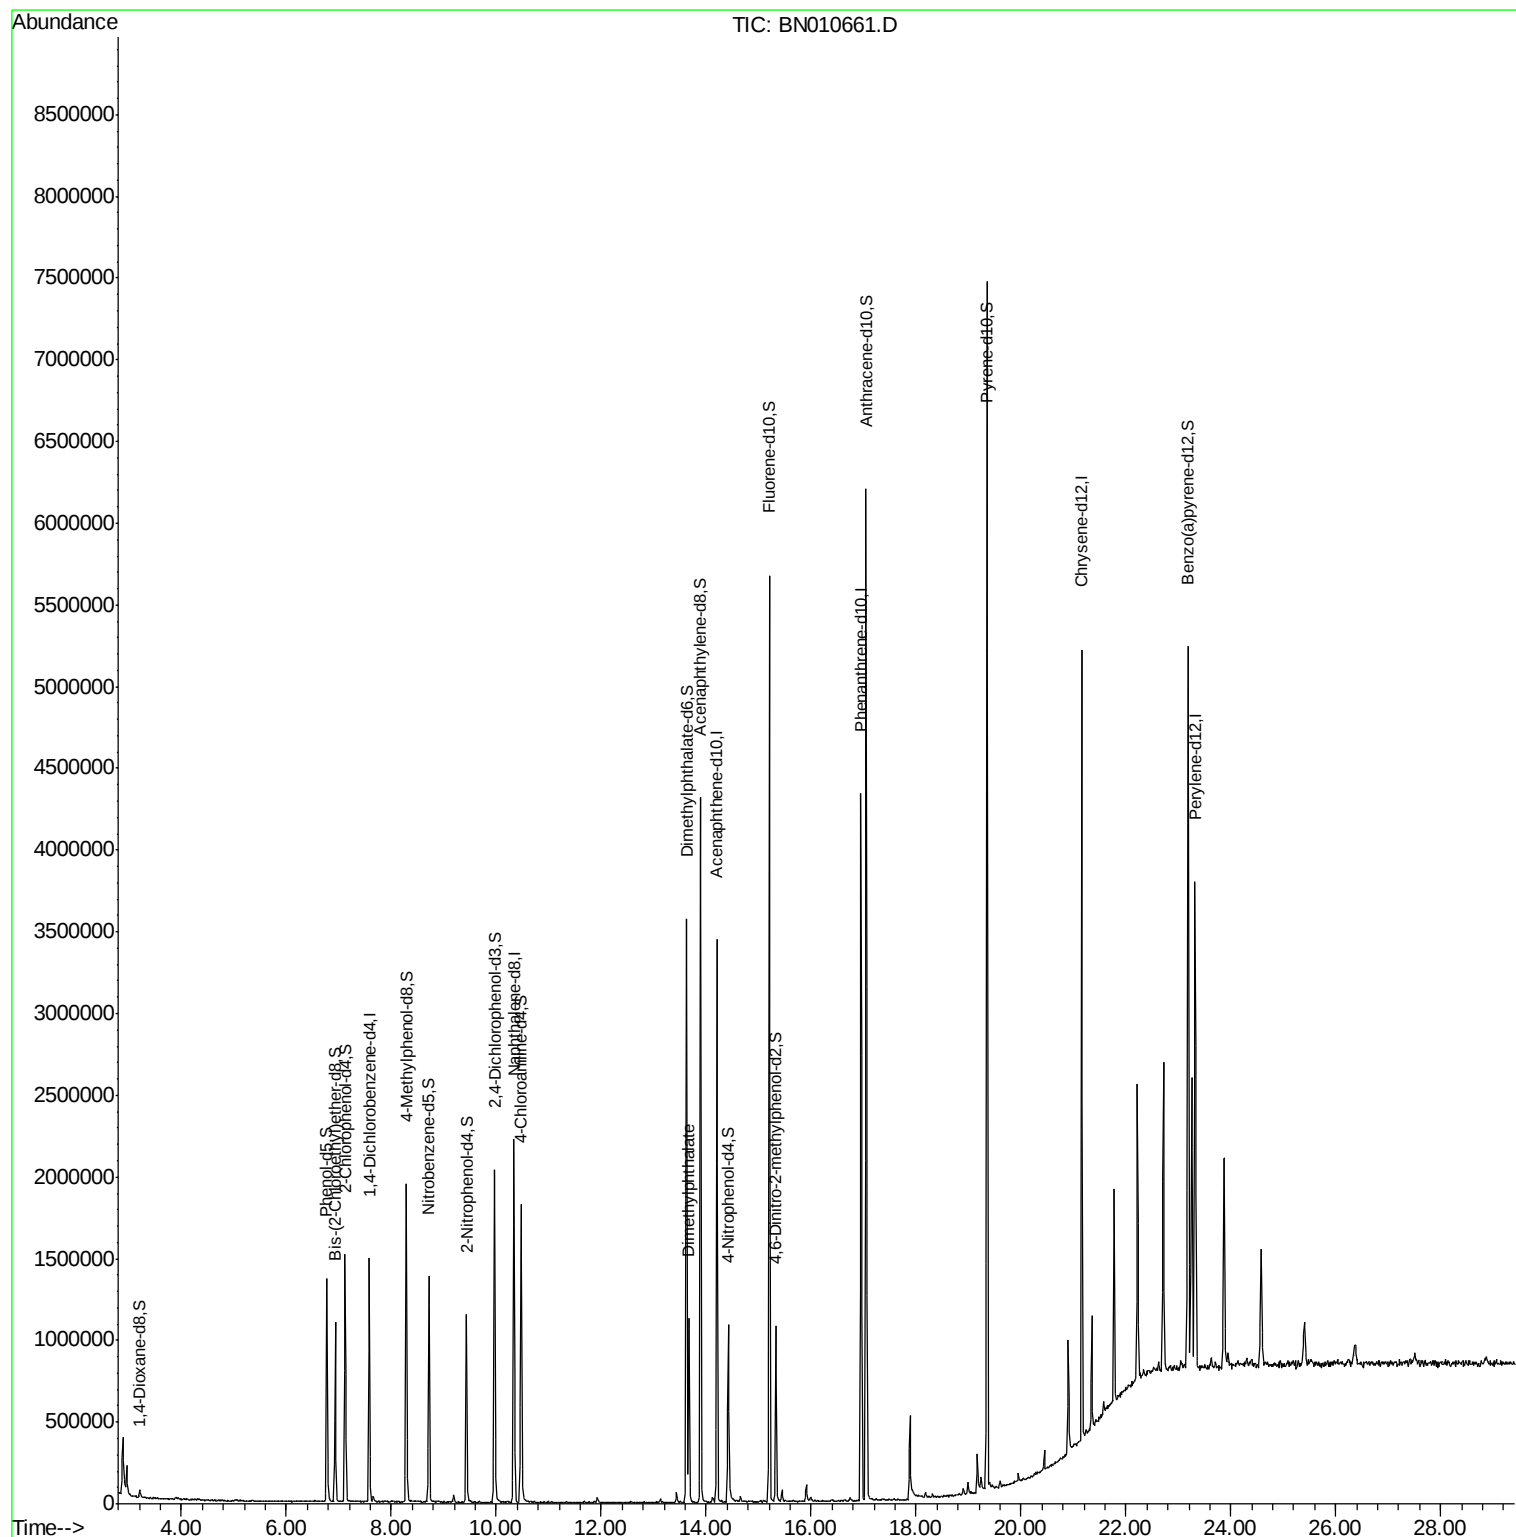

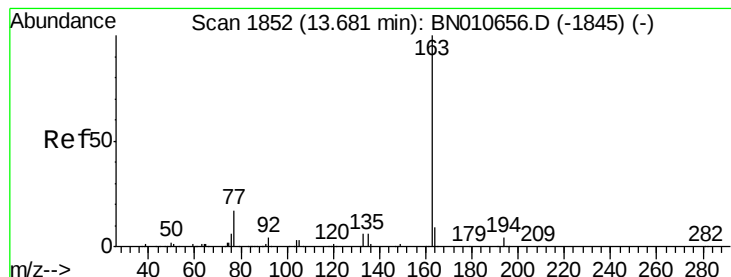

#45

Dimethylphthalate

Concen: 8.09 ng/ul

RT: 13.67 min Scan# 1850

Delta R.T. -0.01 min

Lab File: BN010661.D

Acq: 29 Apr 2020 18:55

Instrument :

BNA_N

ClientSampleId :

C0AF7


Tgt Ion:163 Resp: 722657

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.7 8.0 12.0

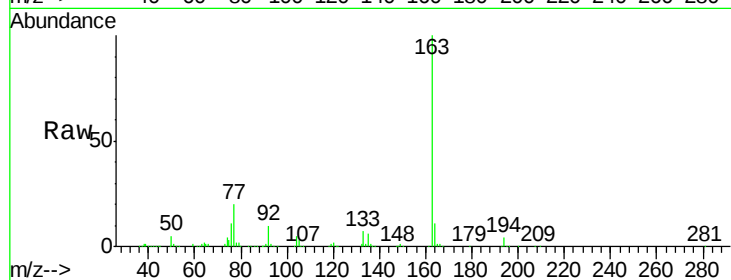

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

