
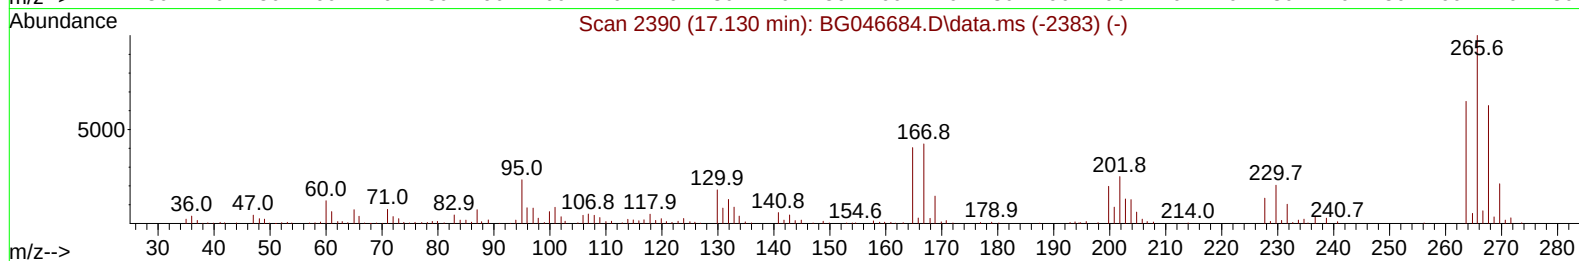
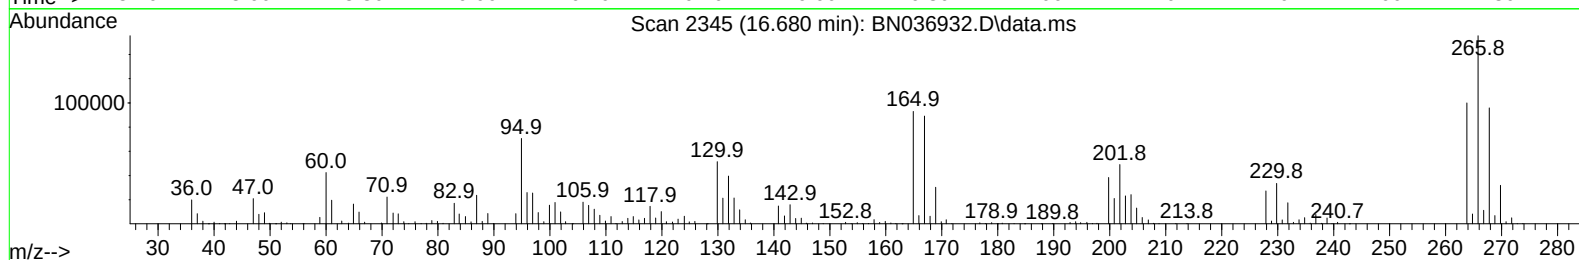


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042925\
Data File : BN036932.D
Acq On : 29 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 17:24:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

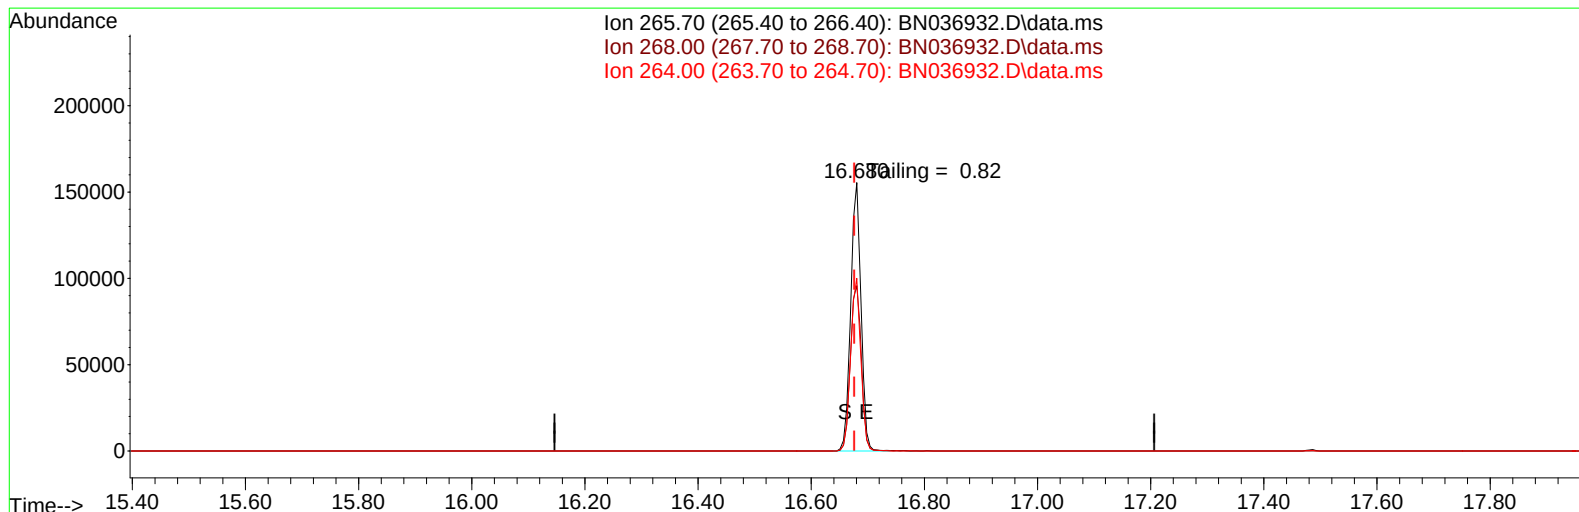

TIC: BN036932.D\data.ms

(70) Pentachlorophenol (C)




16.680min (+ 0.005) 17951.16 ng

response 196804

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.62
264.00	61.60	64.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN042925\
Data File : BN036932.D
Acq On : 29 Apr 2025 08:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 17:26:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

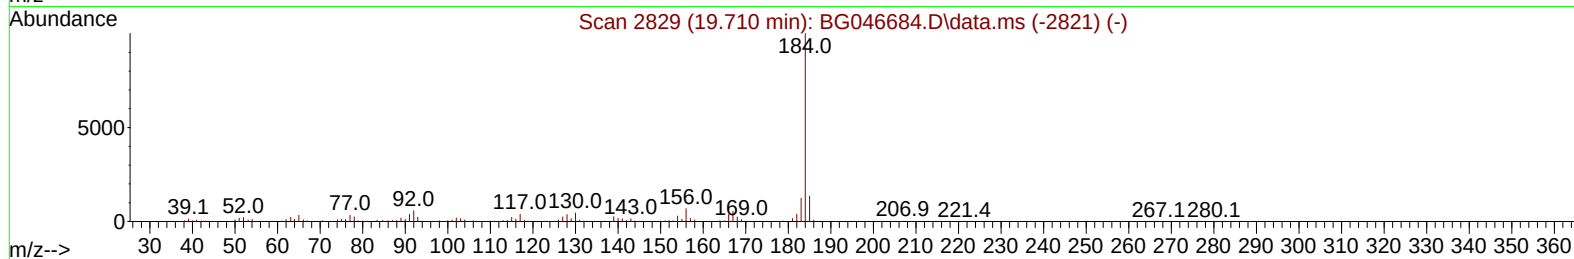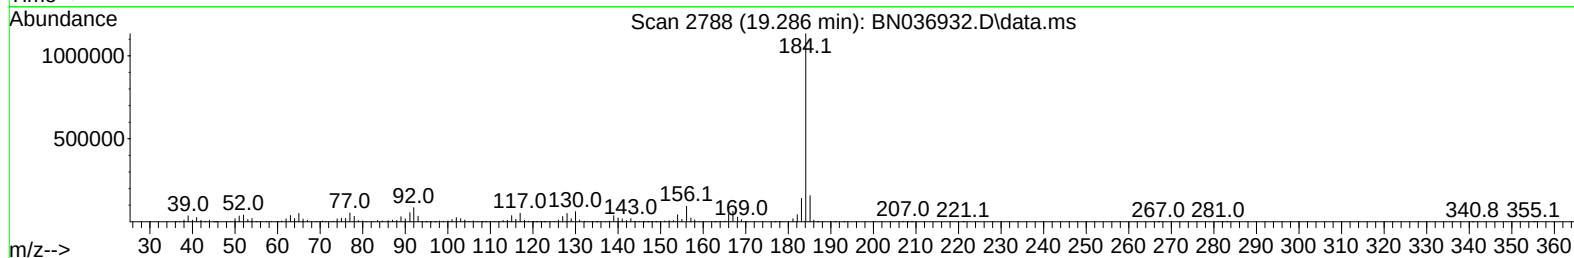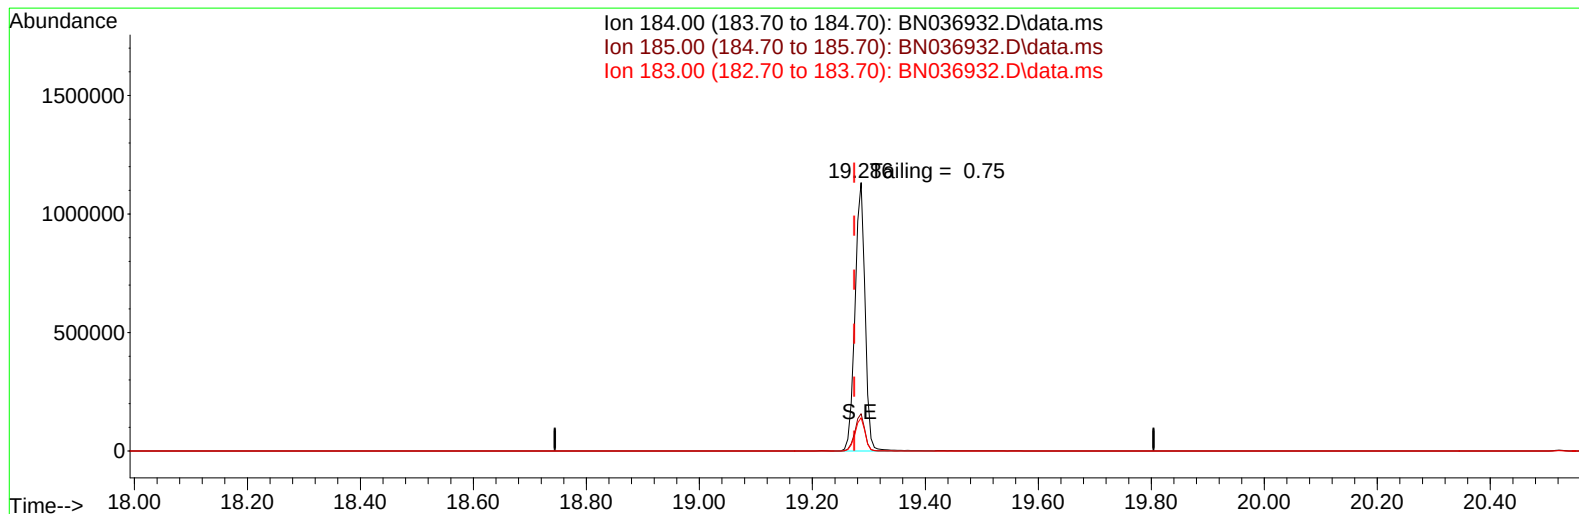

TIC: BN036932.D\data.ms

(77) Benzidine

19.286min (+ 0.012) 0.00 ng

response 1411976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	12.44
0.00	0.00	0.00