

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
 Data File : BN005379.D
 Acq On : 30 Apr 2019 19:39
 Operator : JU/SJ
 Sample : K2596-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: May 01 00:44:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	351343	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1497734	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1002387	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2488660	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	2607113	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2826980	20.00	ng/ul	-0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	28861	3.97	ng/uL	0.00
5) Phenol-d5	6.77	99	582253	21.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	354177	20.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	476113	22.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	493502	22.88	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	254379	27.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	285271	30.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	506913	23.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	685110	31.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1874994	25.77	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	2147450	24.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	246864	21.49	ng/ul	0.00
57) Fluorene-d10	15.22	176	1586573	25.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	246482	22.02	ng/ul	0.00
70) Anthracene-d10	17.07	188	2513260	24.09	ng/ul	-0.01
78) Pyrene-d10	19.39	212	2950837	22.13	ng/ul	-0.01
89) Benzo(a)pyrene-d12	23.26	264	2875290	23.27	ng/ul	-0.04


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	542663	7.485	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
Data File : BN005379.D
Acq On : 30 Apr 2019 19:39
Operator : JU/SJ
Sample : K2596-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: May 01 00:44:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

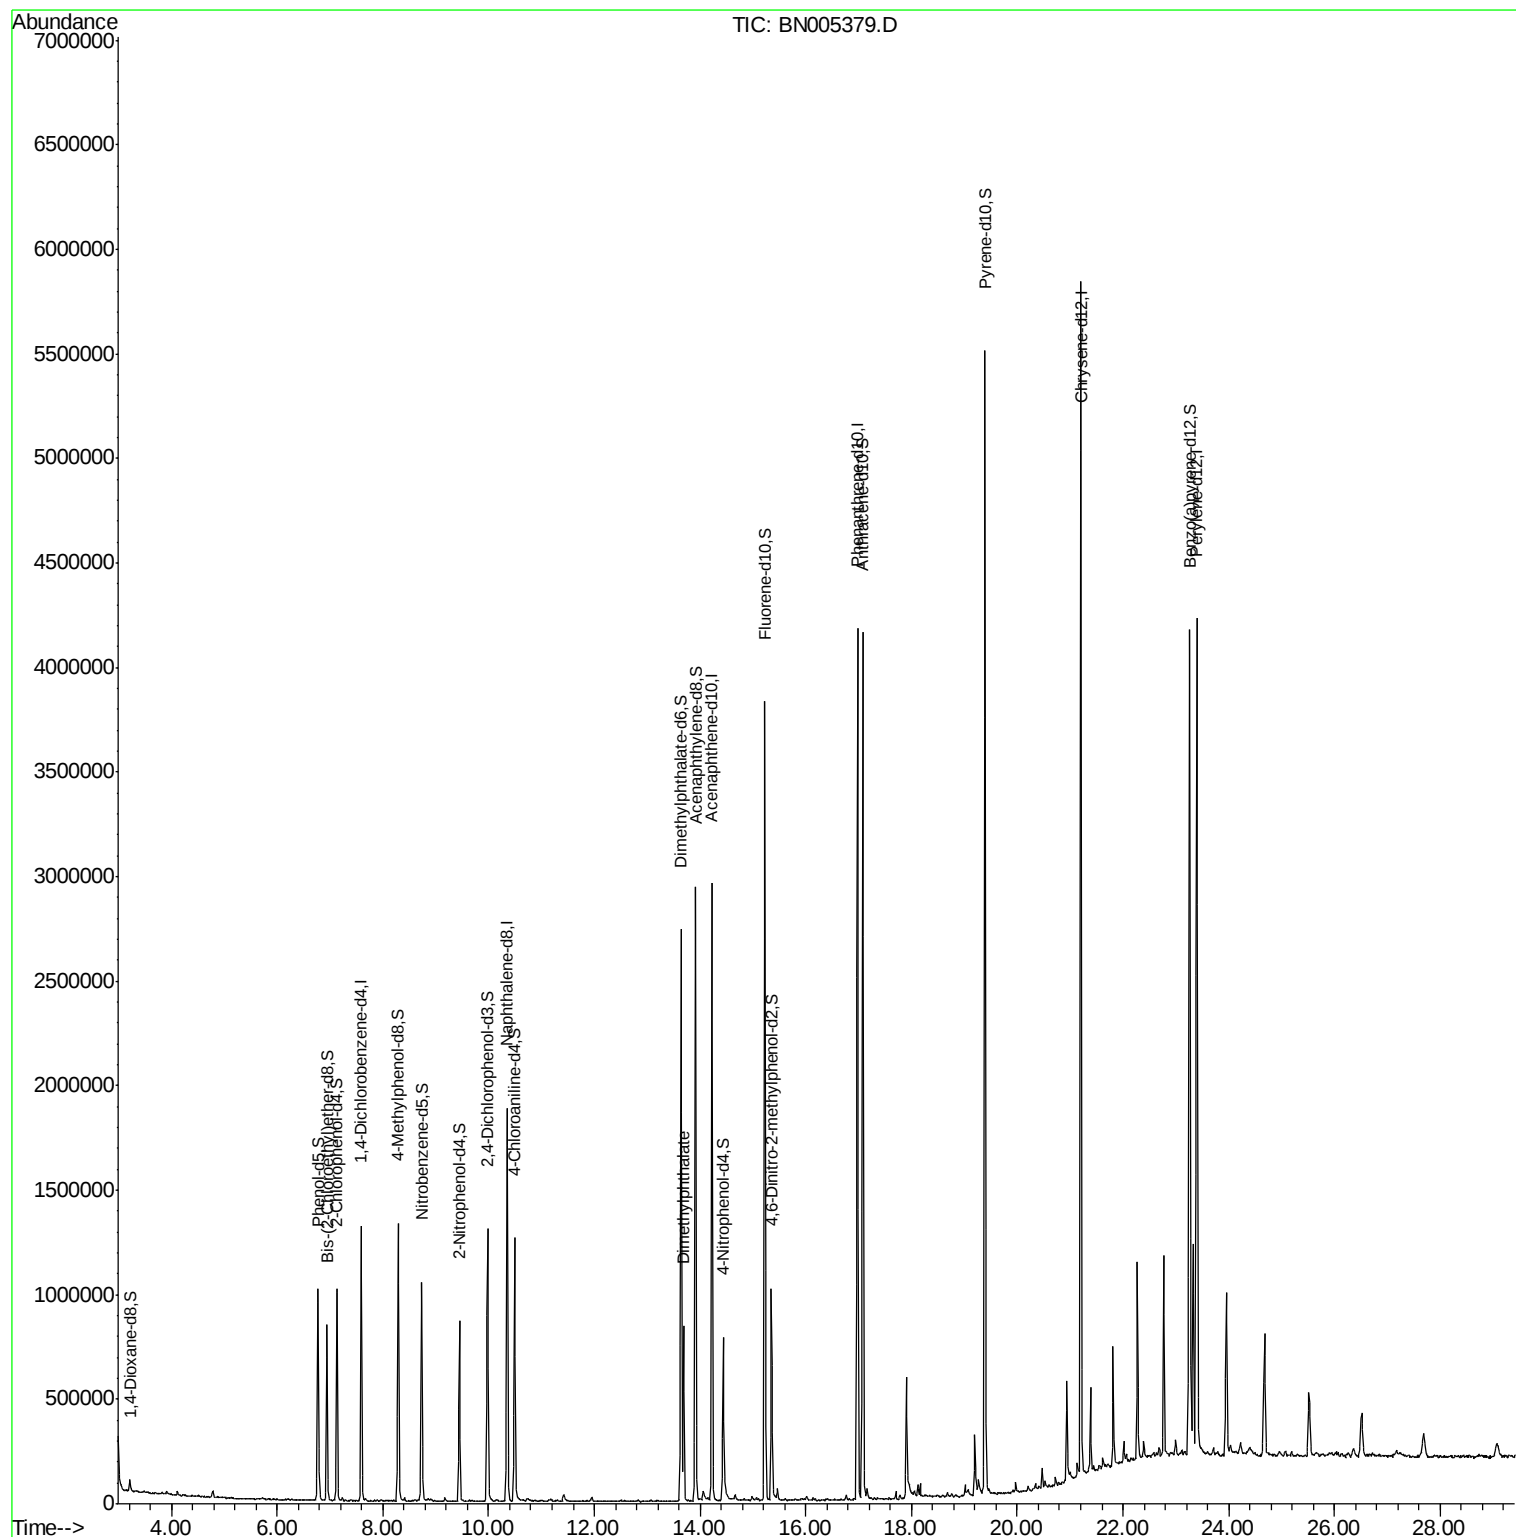

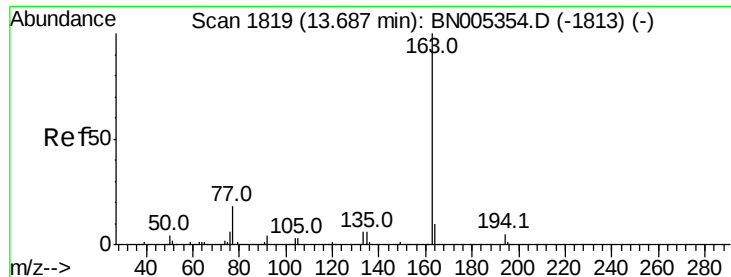

#44

Dimethylphthalate

Concen: 7.485 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN005379.D

Acq: 30 Apr 2019 19:39

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 542663

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.9 8.1 12.1

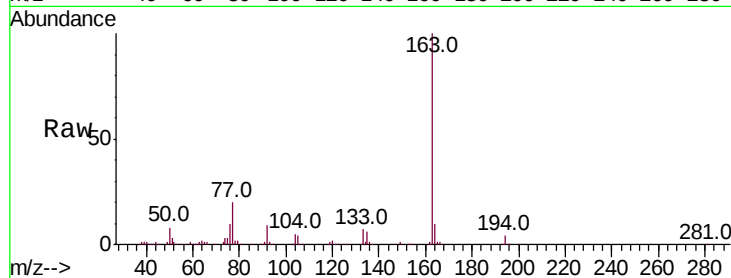

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

