

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
 Data File : BN005371.D
 Acq On : 30 Apr 2019 15:01
 Operator : JU/SJ
 Sample : K2470-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5137

Quant Time: May 01 00:43:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	300553	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1280216	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.22	164	862058	20.00	ng/ul	-0.01
61) Phenanthrene-d10	16.98	188	2110352	20.00	ng/ul	0.00
77) Chrysene-d12	21.21	240	2201941	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2413132	20.00	ng/ul	-0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	19784	3.18	ng/uL	0.00
5) Phenol-d5	6.78	99	544476	23.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	314301	21.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	435792	24.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	447675	24.26	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	225515	28.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	264084	33.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	451441	24.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	598964	31.72	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1606982	25.68	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1929612	25.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.43	143	244782	24.77	ng/ul	0.00
57) Fluorene-d10	15.23	176	1373823	26.16	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	201287	21.21	ng/ul	0.00
70) Anthracene-d10	17.07	188	2234409	25.26	ng/ul	-0.01
78) Pyrene-d10	19.39	212	2634892	23.39	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.27	264	2626398	24.90	ng/ul	-0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.69	163	419056	6.721	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN043019\
Data File : BN005371.D
Acq On : 30 Apr 2019 15:01
Operator : JU/SJ
Sample : K2470-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5137

Quant Time: May 01 00:43:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

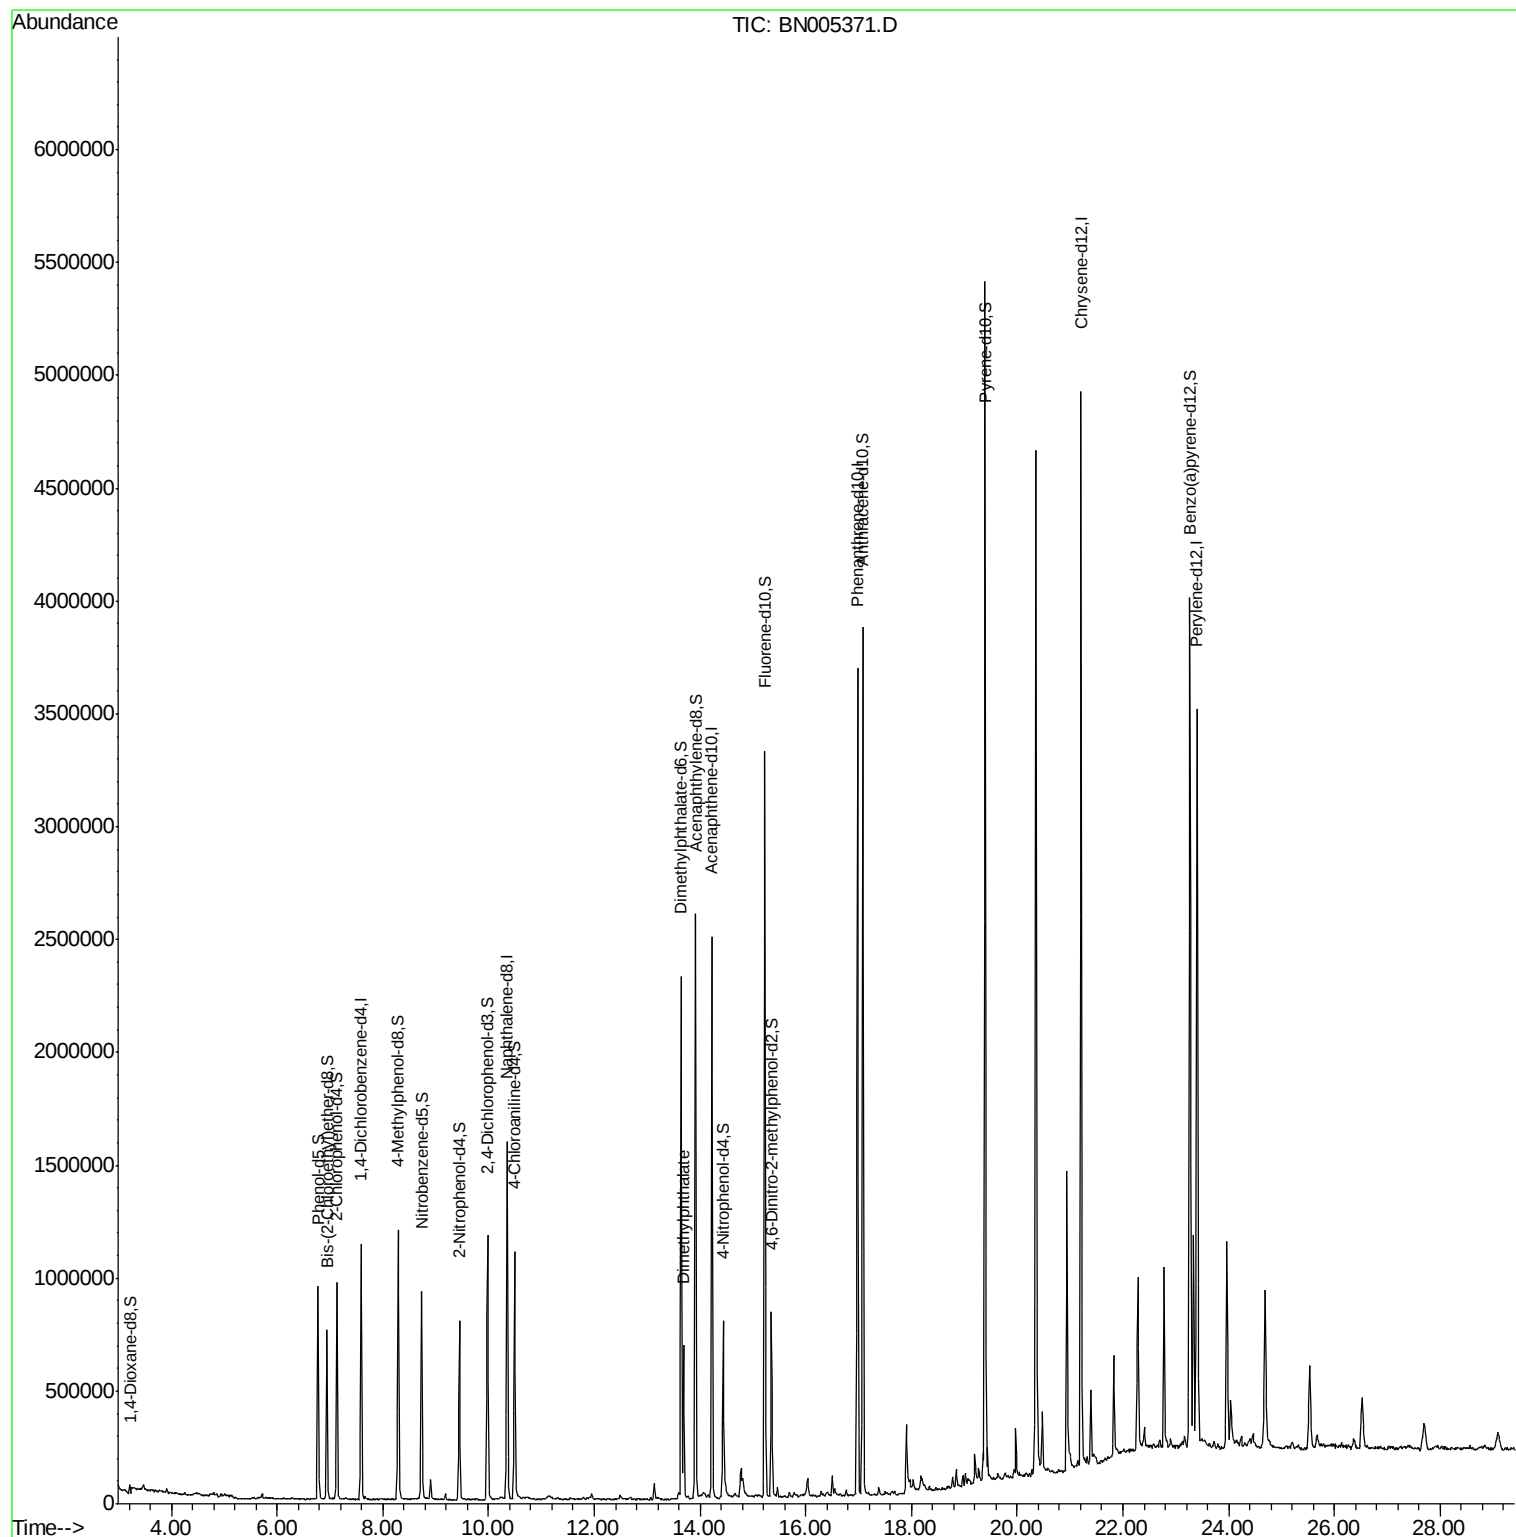

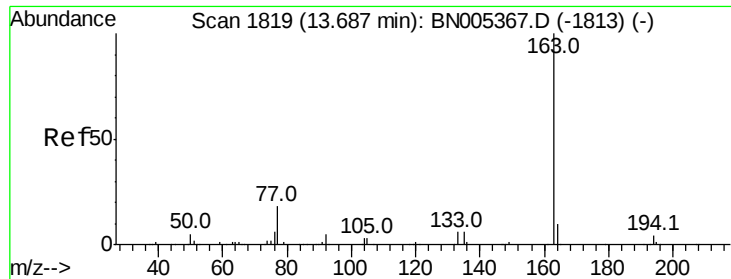

#44

Dimethylphthalate

Concen: 6.721 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN005371.D

Acq: 30 Apr 2019 15:01

Instrument :

BNA_N

ClientSampleId :

A5137


Tot Ion:163 Resp: 419056

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.7 8.1 12.1

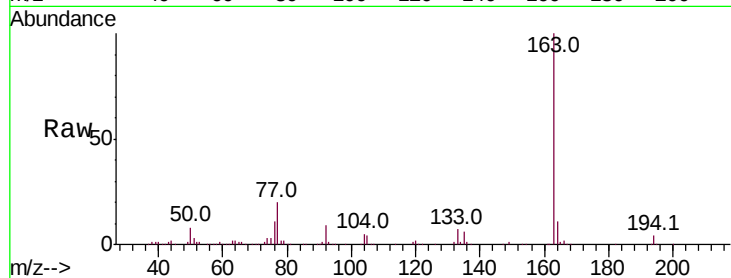

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

