

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
 Data File : BN005381.D
 Acq On : 30 Apr 2019 20:48
 Operator : JU/SJ
 Sample : K2596-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH51

Quant Time: May 01 00:44:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	337846	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	1480444	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	977679	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	2369603	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	2481712	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2672223	20.00	ng/ul	-0.04

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.22	96	22523	3.22	ng/uL	0.00
5) Phenol-d5	6.78	99	488533	18.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	292528	17.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	391640	19.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	411775	19.85	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	206731	22.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	234424	25.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	421378	19.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	527408	24.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.65	166	1559345	21.97	ng/ul	0.00
46) Acenaphthylene-d8	13.92	160	1779232	20.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.44	143	259086	23.12	ng/ul	0.00
57) Fluorene-d10	15.22	176	1284301	21.56	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	235213	22.07	ng/ul	0.00
70) Anthracene-d10	17.07	188	2095081	21.09	ng/ul	-0.01
78) Pyrene-d10	19.39	212	2472922	19.48	ng/ul	-0.01
89) Benzo(a)pyrene-d12	23.26	264	2450095	20.98	ng/ul	-0.04


Target Compounds					Ovalue	
44) Dimethylphthalate	13.69	163	439698	6.218	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
Data File : BN005381.D
Acq On : 30 Apr 2019 20:48
Operator : JU/SJ
Sample : K2596-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFH51

Quant Time: May 01 00:44:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

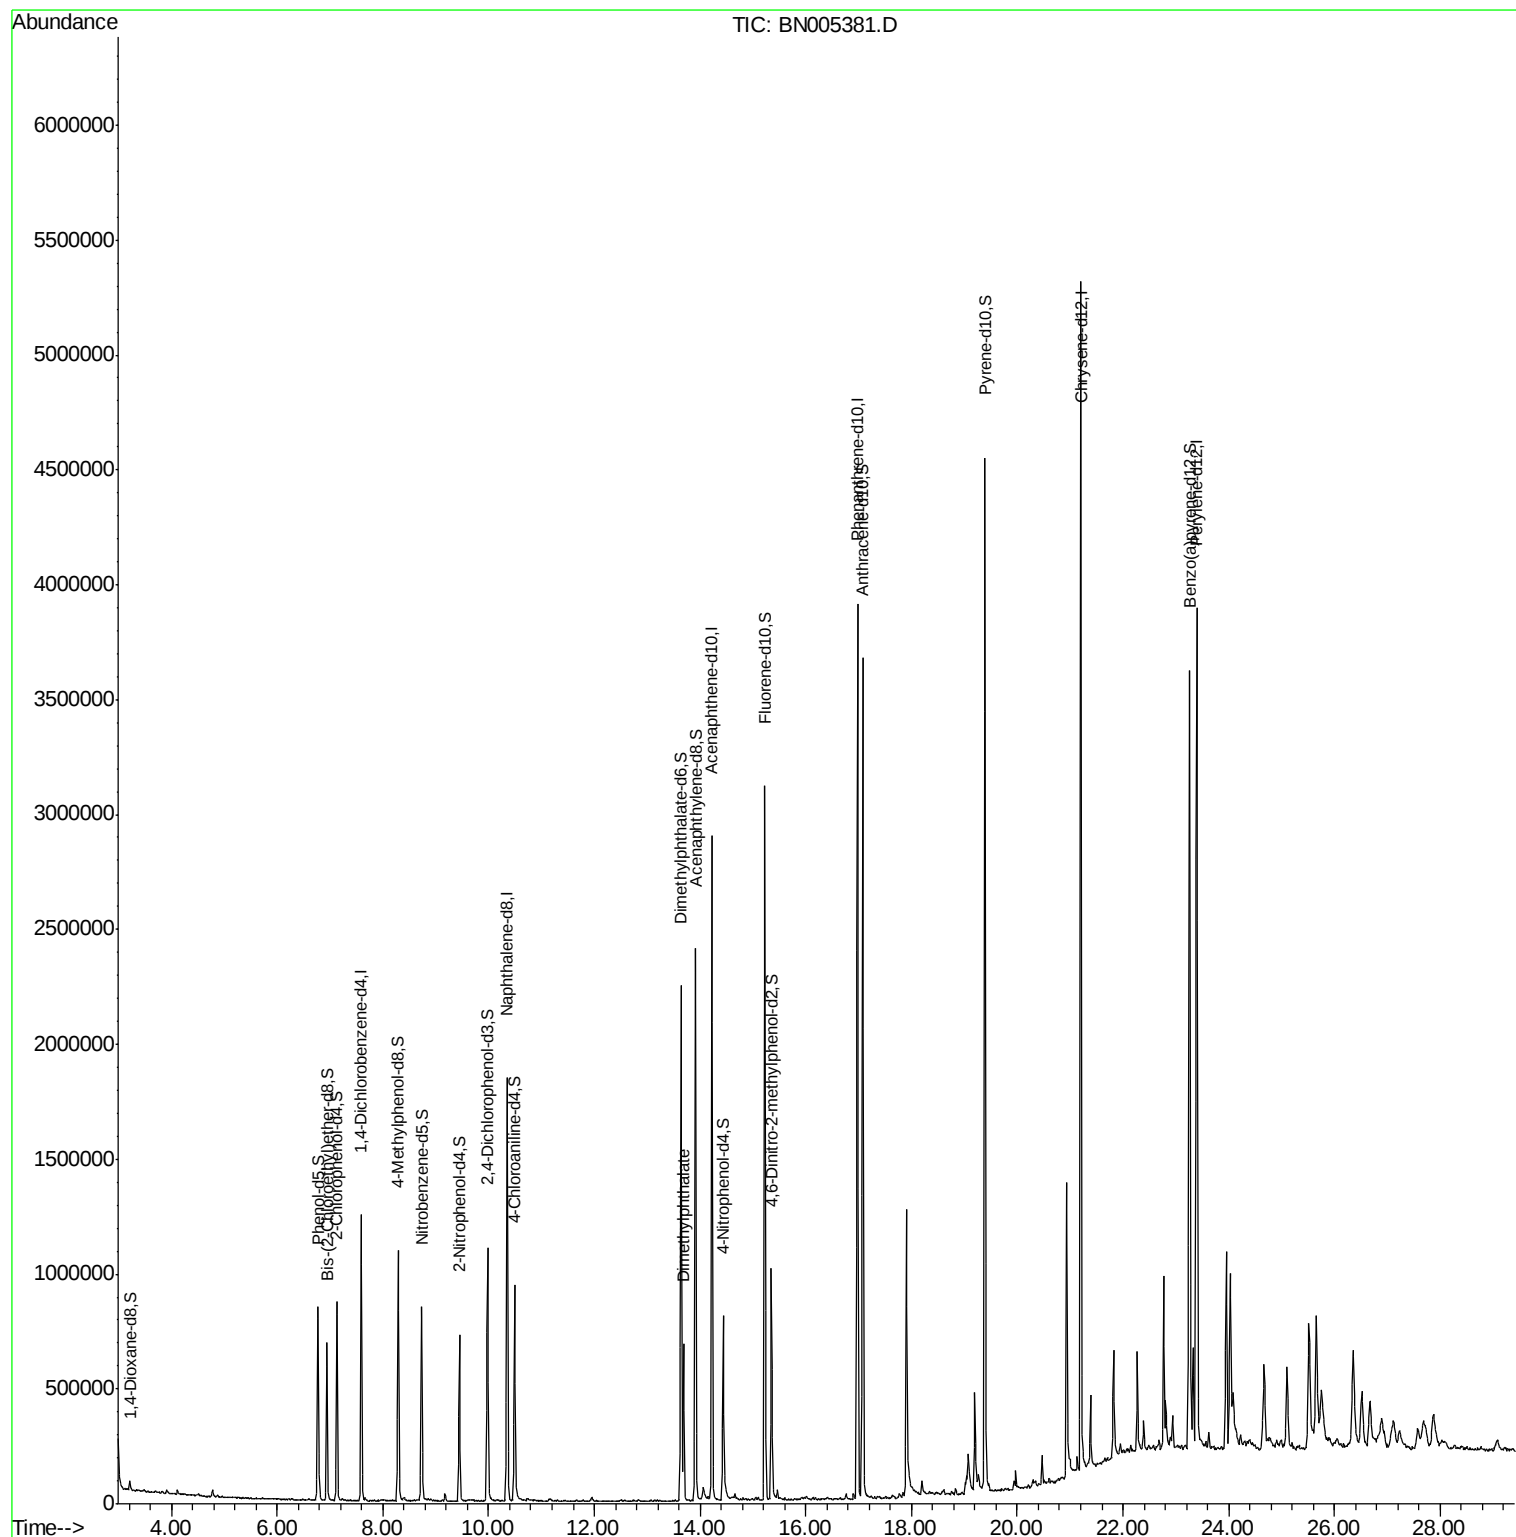

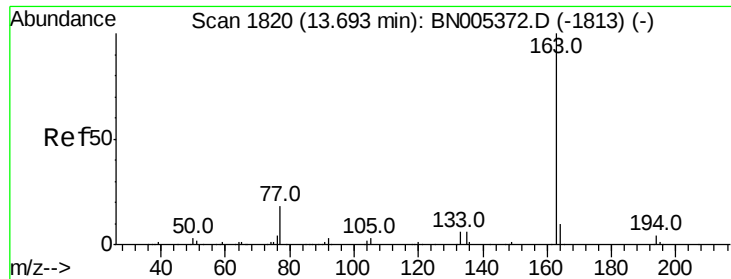

#44

Dimethylphthalate

Concen: 6.218 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN005381.D

Acq: 30 Apr 2019 20:48

Instrument :

BNA_N

ClientSampleId :

BFH51


Tot Ion:163 Resp: 439698

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 10.5 8.1 12.1

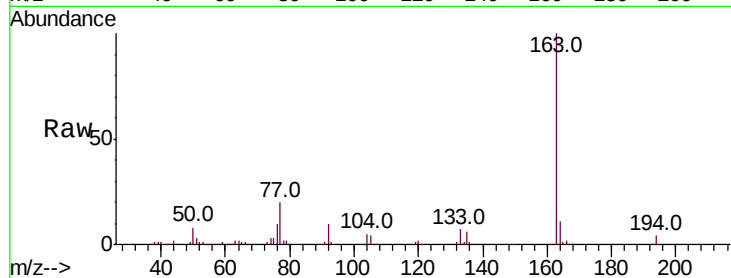

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

