

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043019\
 Data File : BN005393.D
 Acq On : 01 May 2019 04:19
 Operator : JU/SJ
 Sample : K2596-04 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFH40

Quant Time: May 01 07:46:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 25 03:19:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	546657	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	2322532	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.23	164	1408837	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.98	188	3100750	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	2225548	20.00	ng/ul	-0.02
85) Perylene-d12	23.40	264	2183261	20.00	ng/ul	-0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	8566	0.76	ng/uL	0.00
5) Phenol-d5	6.78	99	211241	4.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.94	67	115112	4.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.13	132	171264	5.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	174420	5.20	ng/ul	0.00
19) Nitrobenzene-d5	8.73	128	81869	5.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.45	143	91670	6.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.98	165	177240	5.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	161924	4.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.64	166	554182	5.42	ng/ul	-0.01
46) Acenaphthylene-d8	13.92	160	683845	5.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	63060	3.91	ng/ul	0.01
57) Fluorene-d10	15.22	176	483397	5.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	44104	3.16	ng/ul	0.00
70) Anthracene-d10	17.07	188	731931	5.63	ng/ul	-0.01
78) Pyrene-d10	19.39	212	739551	6.50	ng/ul	-0.01
89) Benzo(a)pyrene-d12	23.26	264	534862	5.61	ng/ul	-0.04

Target Compounds


					Ovalue	
44) Dimethylphthalate	13.69	163	143822	1.411	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN043019\
Data File : BN005393.D
Acq On : 01 May 2019 04:19
Operator : JU/SJ
Sample : K2596-04 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFH40

Quant Time: May 01 07:46:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 25 03:19:34 2019
Response via : Initial Calibration

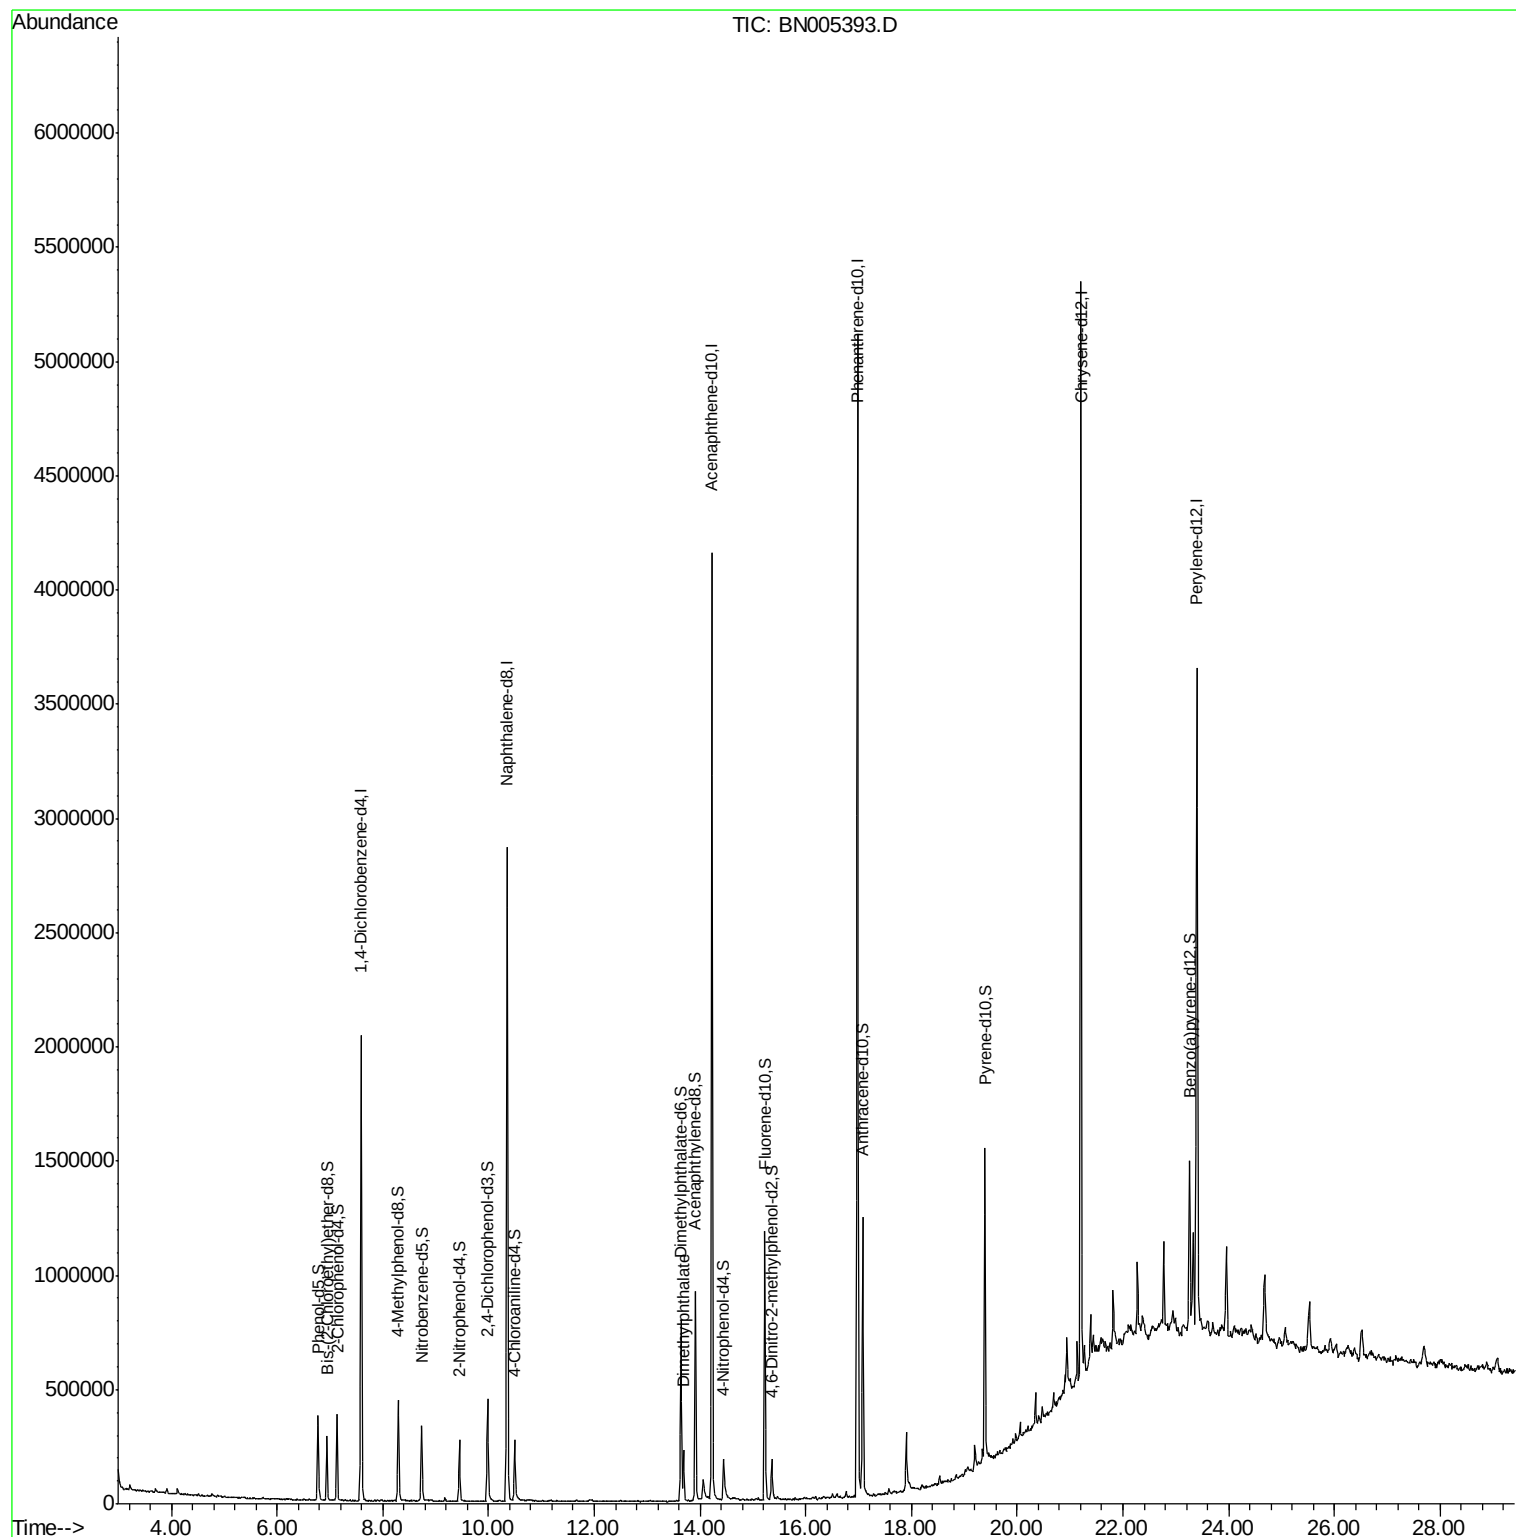

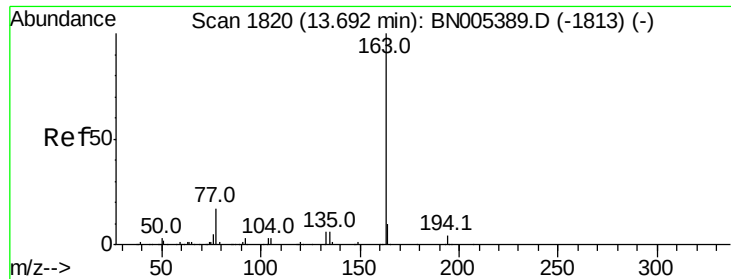

#44

Dimethylphthalate

Concen: 1.411 ng/ul

RT: 13.69 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BN005393.D

Acq: 01 May 2019 04:19

Instrument :

BNA_N

ClientSampleId :

BFH40


Tot Ion:163 Resp: 143822

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.0

164 9.3 8.1 12.1

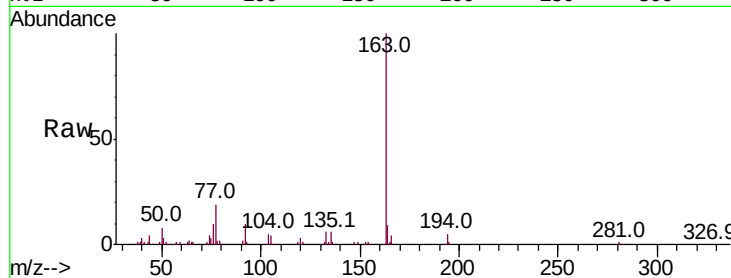

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

