

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN043019\
 Data File : BN005376.D
 Acq On : 30 Apr 2019 17:54
 Operator : JU/SJ
 Sample : PB119273BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	35	39	45	rBV	77338	106539	0.88%	0.094%
2	3.911	154	157	163	rVB5	11575	16677	0.14%	0.015%
3	6.775	637	644	656	rBV	1320758	2101442	17.33%	1.851%
4	6.940	666	672	684	rBV	1048294	1643143	13.55%	1.447%
5	7.128	697	704	717	rBV	1322491	2158532	17.80%	1.901%
6	7.593	776	783	792	rBV	1299886	2097519	17.30%	1.847%
7	8.293	893	902	916	rBV	1681960	2753093	22.70%	2.425%
8	8.734	969	977	986	rBV	1339579	2221189	18.32%	1.956%
9	9.446	1090	1098	1108	rBV	1158000	1917735	15.81%	1.689%
10	9.981	1181	1189	1206	rBV	1683946	2895230	23.88%	2.550%
11	10.351	1243	1252	1260	rBV	1883931	3131196	25.82%	2.758%
12	10.493	1268	1276	1293	rBV	1767038	3114660	25.69%	2.743%
13	11.157	1379	1389	1391	rBV8	7678	15397	0.13%	0.014%
14	11.181	1391	1393	1405	rVB7	7444	14903	0.12%	0.013%
15	11.957	1518	1525	1531	rVB2	23132	50329	0.42%	0.044%
16	13.192	1727	1735	1738	rBV6	5957	13039	0.11%	0.011%
17	13.598	1797	1804	1805	rBV5	18007	23091	0.19%	0.020%
18	13.645	1805	1812	1826	rVB	3913691	5587002	46.07%	4.921%
19	13.916	1850	1858	1869	rBV	4136366	6121635	50.48%	5.391%
20	14.069	1876	1884	1894	rBV4	29069	77366	0.64%	0.068%
21	14.228	1904	1911	1920	rBV2	3098258	4776463	39.39%	4.207%
22	14.434	1937	1946	1970	rBV	1520924	2863584	23.61%	2.522%
23	14.816	2005	2011	2019	rBV4	16322	34371	0.28%	0.030%
24	15.228	2074	2081	2093	rBV	5382013	7785056	64.20%	6.856%
25	15.351	2096	2102	2116	rVV	1801348	2775739	22.89%	2.445%
26	15.463	2117	2121	2127	rVB	72255	109921	0.91%	0.097%
27	15.910	2191	2197	2200	rBV6	7298	12319	0.10%	0.011%
28	16.016	2210	2215	2225	rBV8	24456	59448	0.49%	0.052%
29	16.657	2321	2324	2328	rBV5	10589	13110	0.11%	0.012%
30	16.763	2335	2342	2349	rBV3	18960	31770	0.26%	0.028%
31	16.980	2372	2379	2389	rBV	4575031	6379367	52.61%	5.618%
32	17.080	2389	2396	2411	rVV	6348904	9233917	76.15%	8.132%
33	17.898	2531	2535	2541	rBV4	45077	78099	0.64%	0.069%
34	19.022	2721	2726	2732	rBV	73974	103722	0.86%	0.091%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005376.D
Acq On : 30 Apr 2019 17:54
Operator : JU/SJ
Sample : PB119273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK73

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	19.198	2753	2756	2762	rBV5	17816	27802	0.23%	0.024%
36	19.274	2765	2769	2777	rVB	69913	99424	0.82%	0.088%
37	19.392	2782	2789	2803	rVV2	8272930	11587819	95.56%	10.205%
38	21.145	3084	3087	3091	rBV2	23052	31522	0.26%	0.028%
39	21.204	3092	3097	3110	rVV	5984989	7903523	65.18%	6.961%
40	21.392	3126	3129	3136	rVB4	52480	77631	0.64%	0.068%
41	21.821	3199	3202	3207	rBV	81203	91173	0.75%	0.080%
42	22.280	3276	3280	3286	rVB	191811	251891	2.08%	0.222%
43	22.686	3347	3349	3355	rVB4	67401	97192	0.80%	0.086%
44	22.774	3360	3364	3372	rVB	268474	386463	3.19%	0.340%
45	23.268	3440	3448	3455	rBV2	6534616	12126128	100.00%	10.680%
46	23.327	3455	3458	3463	rVV	363232	596170	4.92%	0.525%
47	23.404	3463	3471	3491	rVB	4265716	8328712	68.68%	7.335%
48	23.957	3560	3565	3571	rBV	313651	541590	4.47%	0.477%
49	24.686	3683	3689	3700	rVB	296085	627365	5.17%	0.553%
50	25.533	3827	3833	3841	rVB	186151	454012	3.74%	0.400%


Sum of corrected areas: 113545020

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN043019\
Data File : BN005376.D
Acq On : 30 Apr 2019 17:54
Operator : JU/SJ
Sample : PB119273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

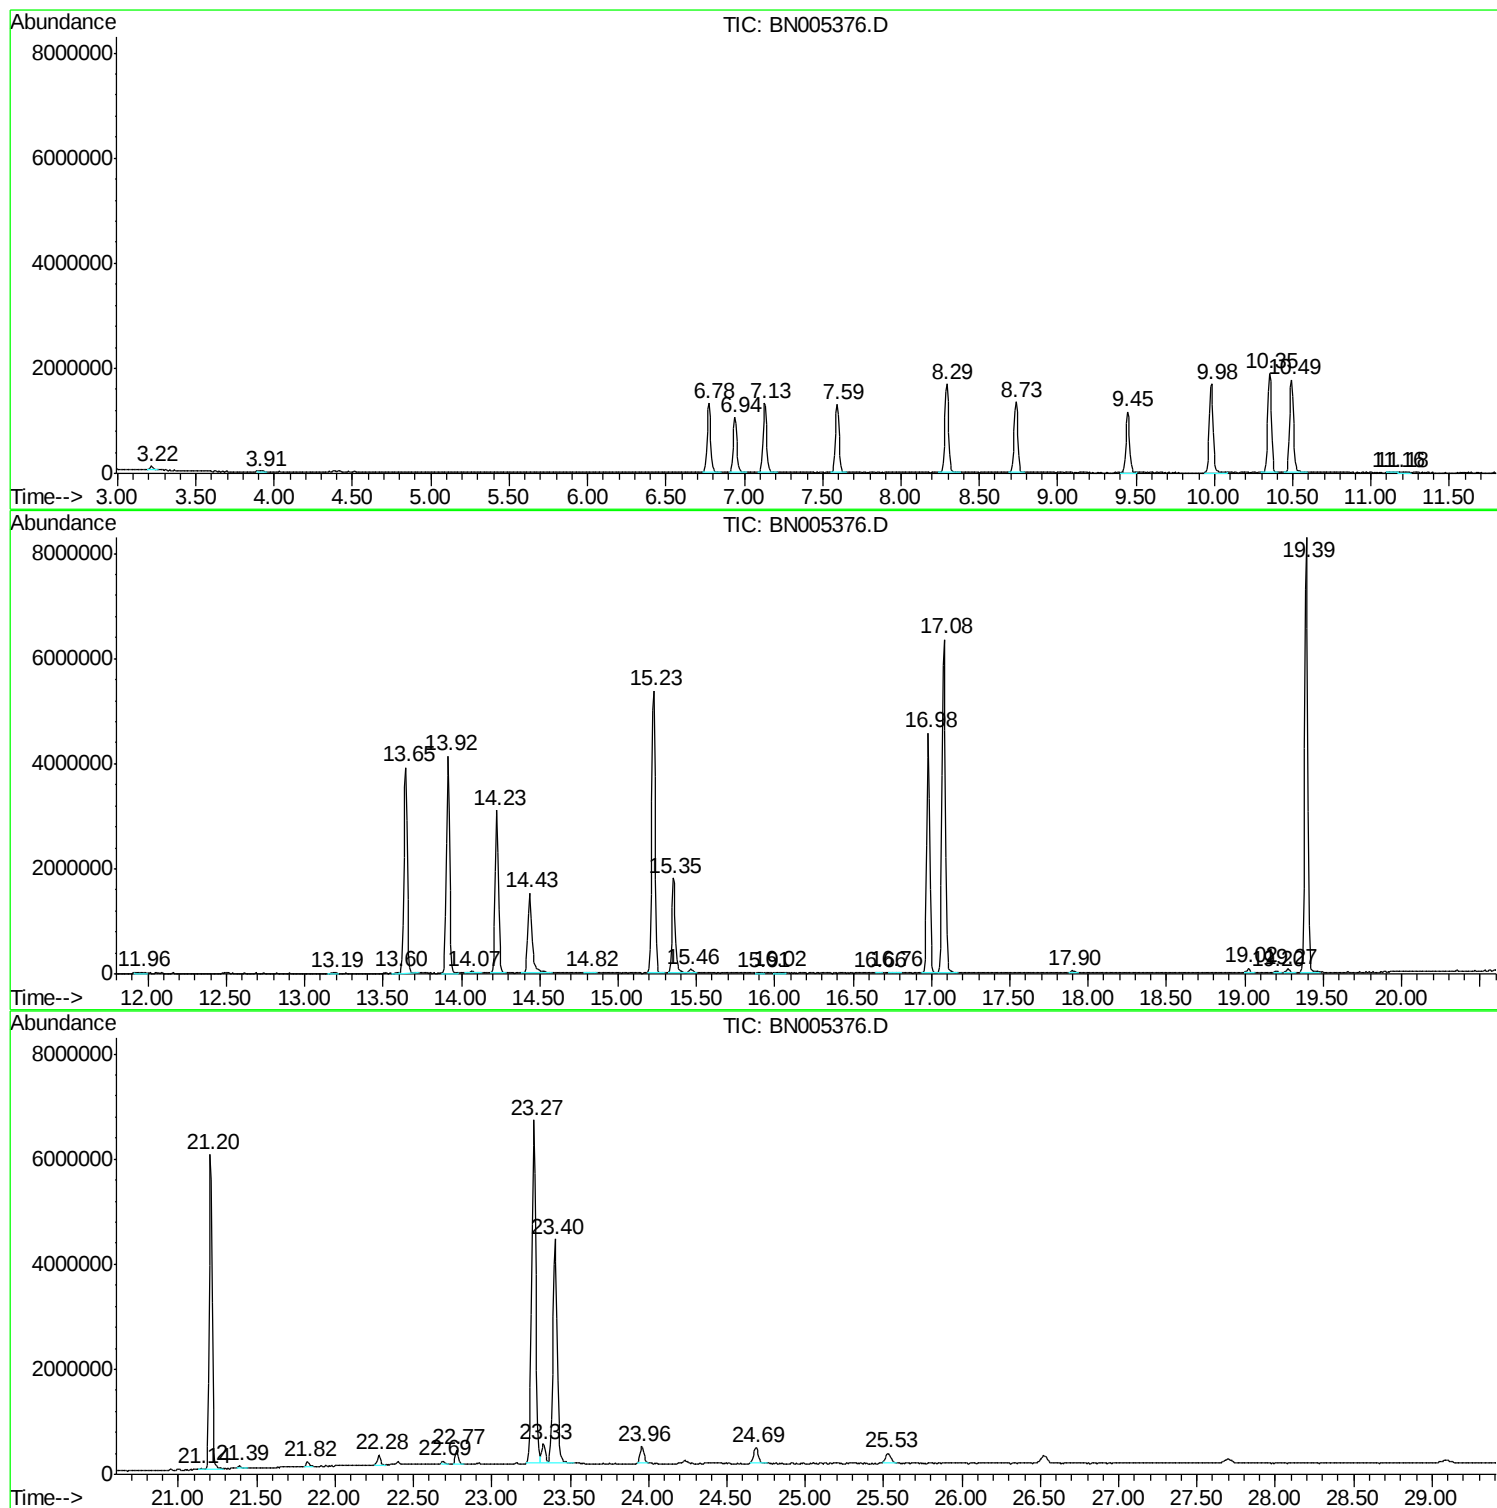

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005376.D
Acq On : 30 Apr 2019 17:54
Operator : JU/SJ
Sample : PB119273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005376.D
Acq On : 30 Apr 2019 17:54
Operator : JU/SJ
Sample : PB119273BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK73

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc