

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN043019\
 Data File : BN005377.D
 Acq On : 30 Apr 2019 18:29
 Operator : JU/SJ
 Sample : PB119190BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	47	rVB	84584	113612	0.91%	0.094%
2	3.911	154	157	167	rVB3	15605	24912	0.20%	0.021%
3	6.775	636	644	661	rBV	1461438	2311590	18.60%	1.918%
4	6.940	665	672	685	rVB	1180598	1798579	14.47%	1.492%
5	7.128	698	704	714	rVB	1446403	2338307	18.81%	1.940%
6	7.593	776	783	797	rBV	1420425	2299100	18.50%	1.907%
7	8.293	895	902	913	rBV	1838450	2967102	23.87%	2.462%
8	8.734	969	977	985	rBV	1473835	2418372	19.46%	2.006%
9	9.446	1090	1098	1107	rBV	1249258	2070351	16.66%	1.718%
10	9.975	1181	1188	1202	rBV	1780766	3153212	25.37%	2.616%
11	10.352	1245	1252	1260	rBV	2033413	3379941	27.19%	2.804%
12	10.493	1268	1276	1292	rBV	1879895	3339965	26.87%	2.771%
13	11.957	1519	1525	1531	rVB	26058	46821	0.38%	0.039%
14	12.493	1612	1616	1624	rBV6	6986	14412	0.12%	0.012%
15	13.646	1805	1812	1827	rVB	4341027	5963785	47.98%	4.948%
16	13.916	1850	1858	1869	rBV	4397901	6544552	52.65%	5.430%
17	14.069	1878	1884	1894	rBV	32674	77413	0.62%	0.064%
18	14.228	1903	1911	1924	rVB2	3289771	5081787	40.88%	4.216%
19	14.434	1938	1946	1968	rBV	1642557	3040616	24.46%	2.523%
20	14.810	2007	2010	2014	rBV5	10560	17676	0.14%	0.015%
21	15.228	2074	2081	2093	rBV	5560221	8301677	66.79%	6.887%
22	15.351	2096	2102	2117	rBV	1907072	3009688	24.21%	2.497%
23	15.463	2117	2121	2129	rVB	79246	126961	1.02%	0.105%
24	16.010	2209	2214	2223	rBV4	25007	47477	0.38%	0.039%
25	16.187	2239	2244	2247	rVB5	8906	13603	0.11%	0.011%
26	16.657	2322	2324	2329	rBV4	10989	13727	0.11%	0.011%
27	16.769	2337	2343	2347	rBV	19973	29928	0.24%	0.025%
28	16.981	2372	2379	2388	rBV2	4626229	6699235	53.90%	5.558%
29	17.081	2389	2396	2410	rVB	6631794	9772447	78.62%	8.108%
30	17.898	2531	2535	2540	rBV6	43985	74497	0.60%	0.062%
31	18.957	2710	2715	2720	rBV6	9224	16525	0.13%	0.014%
32	19.022	2722	2726	2731	rVB	84750	108862	0.88%	0.090%
33	19.198	2752	2756	2759	rBV3	20634	34573	0.28%	0.029%
34	19.275	2764	2769	2775	rVB	80958	109044	0.88%	0.090%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005377.D
Acq On : 30 Apr 2019 18:29
Operator : JU/SJ
Sample : PB119190BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	19.392	2782	2789	2799	rBV	8762238	12211972	98.25%	10.132%
36	20.604	2993	2995	3000	rBV5	14346	19938	0.16%	0.017%
37	21.145	3084	3087	3091	rBV4	24360	36751	0.30%	0.030%
38	21.204	3091	3097	3110	rBV	6302178	8212346	66.07%	6.813%
39	21.392	3126	3129	3135	rVB3	57797	77571	0.62%	0.064%
40	21.822	3199	3202	3210	rVB	107157	135162	1.09%	0.112%
41	22.275	3276	3279	3285	rVB	214449	283481	2.28%	0.235%
42	22.398	3298	3300	3305	rVB2	49756	60019	0.48%	0.050%
43	22.686	3346	3349	3357	rVB4	66651	108290	0.87%	0.090%
44	22.775	3359	3364	3370	rBV	316571	463134	3.73%	0.384%
45	23.269	3439	3448	3455	rBV2	6465747	12430004	100.00%	10.312%
46	23.327	3455	3458	3463	rVV2	418094	681028	5.48%	0.565%
47	23.404	3463	3471	3489	rVB	4240369	8254629	66.41%	6.848%
48	23.957	3560	3565	3572	rVB	350933	619178	4.98%	0.514%
49	24.686	3683	3689	3698	rVB	322581	686033	5.52%	0.569%
50	25.527	3826	3832	3843	rVB	219987	509182	4.10%	0.422%
51	26.515	3996	4000	4011	rVB3	144825	385614	3.10%	0.320%


Sum of corrected areas: 120534681

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN043019\
Data File : BN005377.D
Acq On : 30 Apr 2019 18:29
Operator : JU/SJ
Sample : PB119190BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

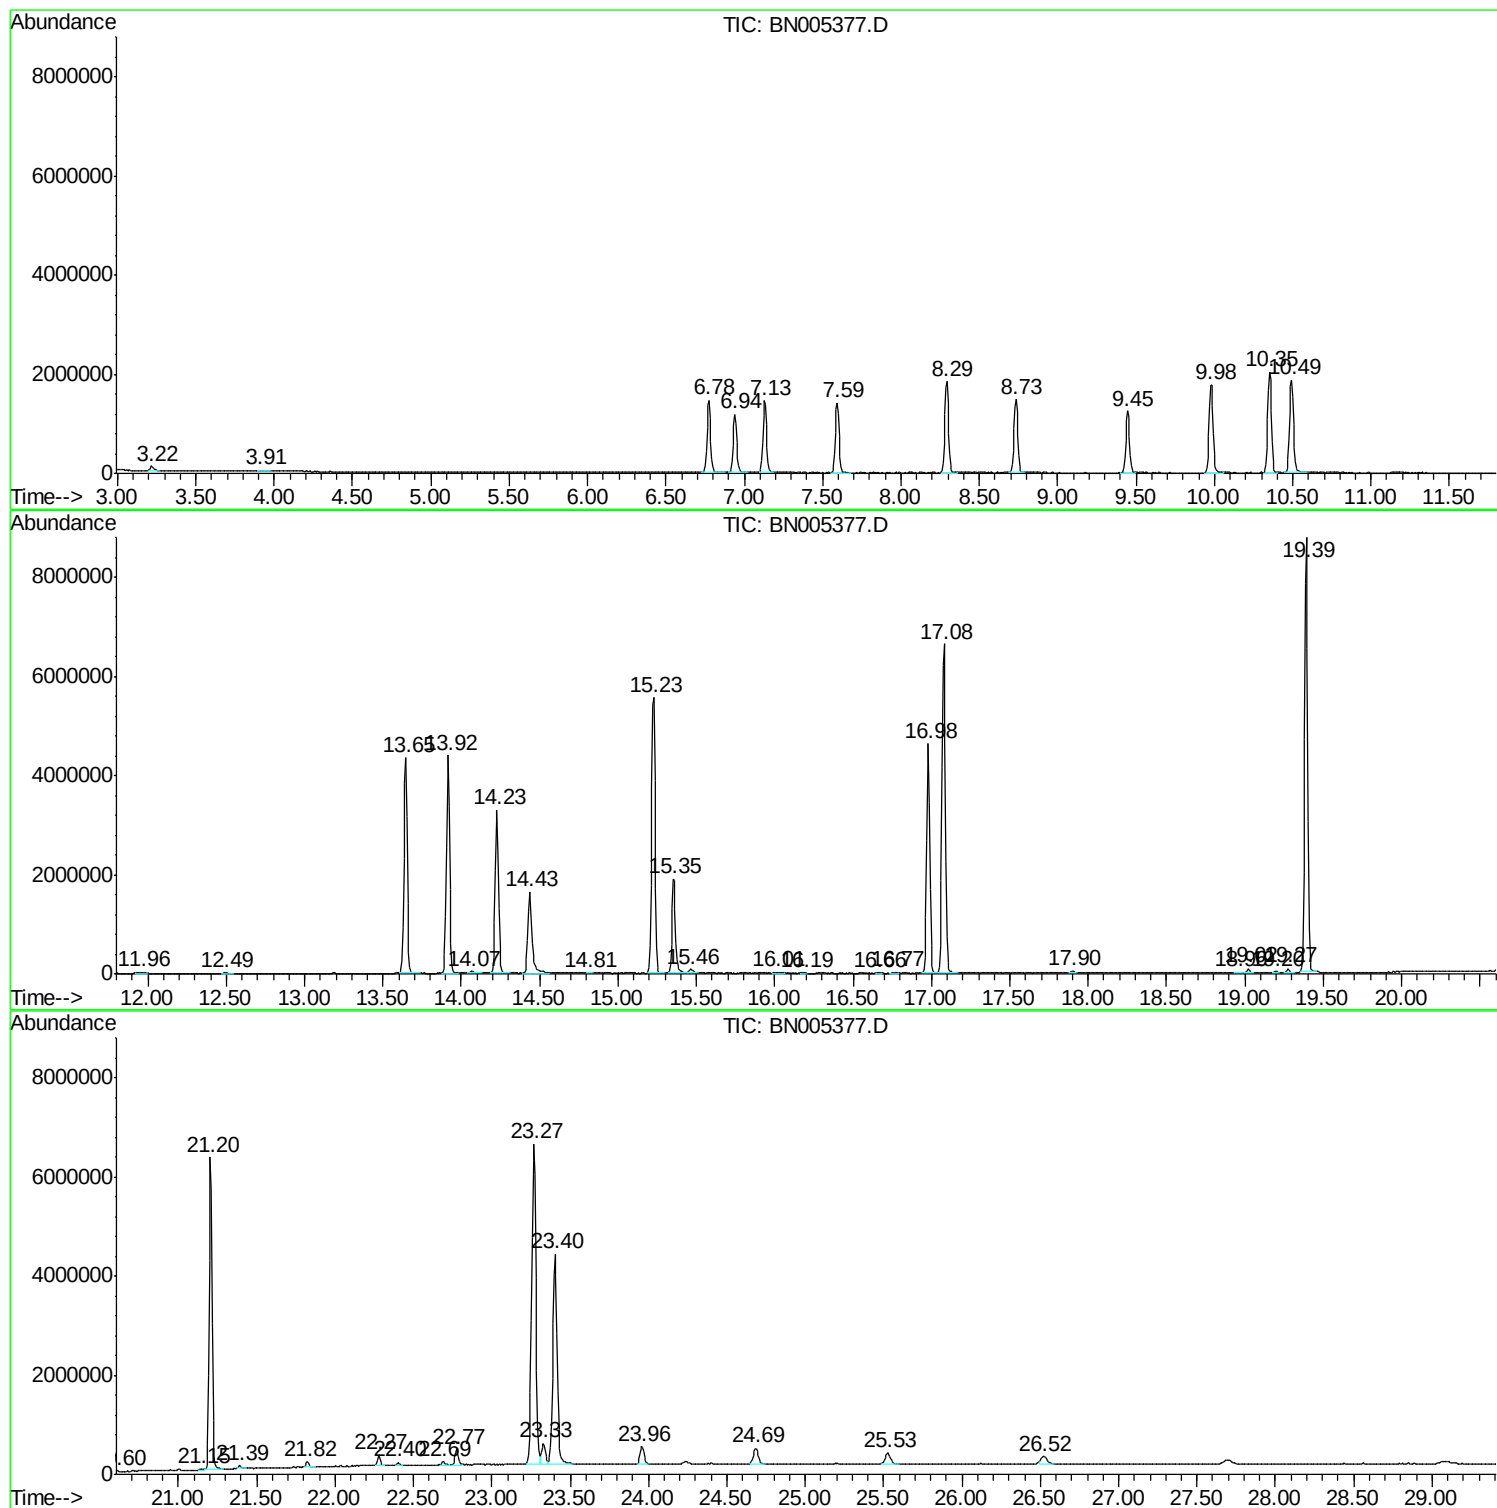

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005377.D
Acq On : 30 Apr 2019 18:29
Operator : JU/SJ
Sample : PB119190BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043019\
Data File : BN005377.D
Acq On : 30 Apr 2019 18:29
Operator : JU/SJ
Sample : PB119190BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc