

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN043020\
 Data File : BN010672.D
 Acq On : 30 Apr 2020 13:50
 Operator : CG/JU
 Sample : PB128575BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB128575BL

Quant Time: Apr 30 14:30:05 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 30 11:18:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3023	0.40	ng	0.00
7) Naphthalene-d8	10.34	136	12115	0.40	ng	0.01
13) Acenaphthene-d10	14.21	164	7490	0.40	ng	0.01
19) Phenanthrene-d10	16.97	188	16324	0.40	ng	0.02
27) Chrysene-d12	21.17	240	11647	0.40	ng	0.01
34) Perylene-d12	23.34	264	10496	0.40	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.23	112	2389	0.36	ng	0.00
5) Phenol-d6	6.78	99	2685	0.31	ng	0.00
8) Nitrobenzene-d5	8.73	82	3020	0.36	ng	0.01
11) 2-Methylnaphthalene-d10	11.94	152	7000	0.35	ng	0.01
14) 2,4,6-Tribromophenol	15.74	330	784	0.22	ng	0.03
15) 2-Fluorobiphenyl	12.84	172	9431	0.35	ng	0.02
25) Fluoranthene-d10	19.00	212	14414	0.29	ng	0.01
29) Terphenyl-d14	19.61	244	10768	0.40	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN043020\
Data File : BN010672.D
Acq On : 30 Apr 2020 13:50
Operator : CG/JU
Sample : PB128575BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB128575BL

Quant Time: Apr 30 14:30:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN041320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 30 11:18:31 2020
Response via : Initial Calibration

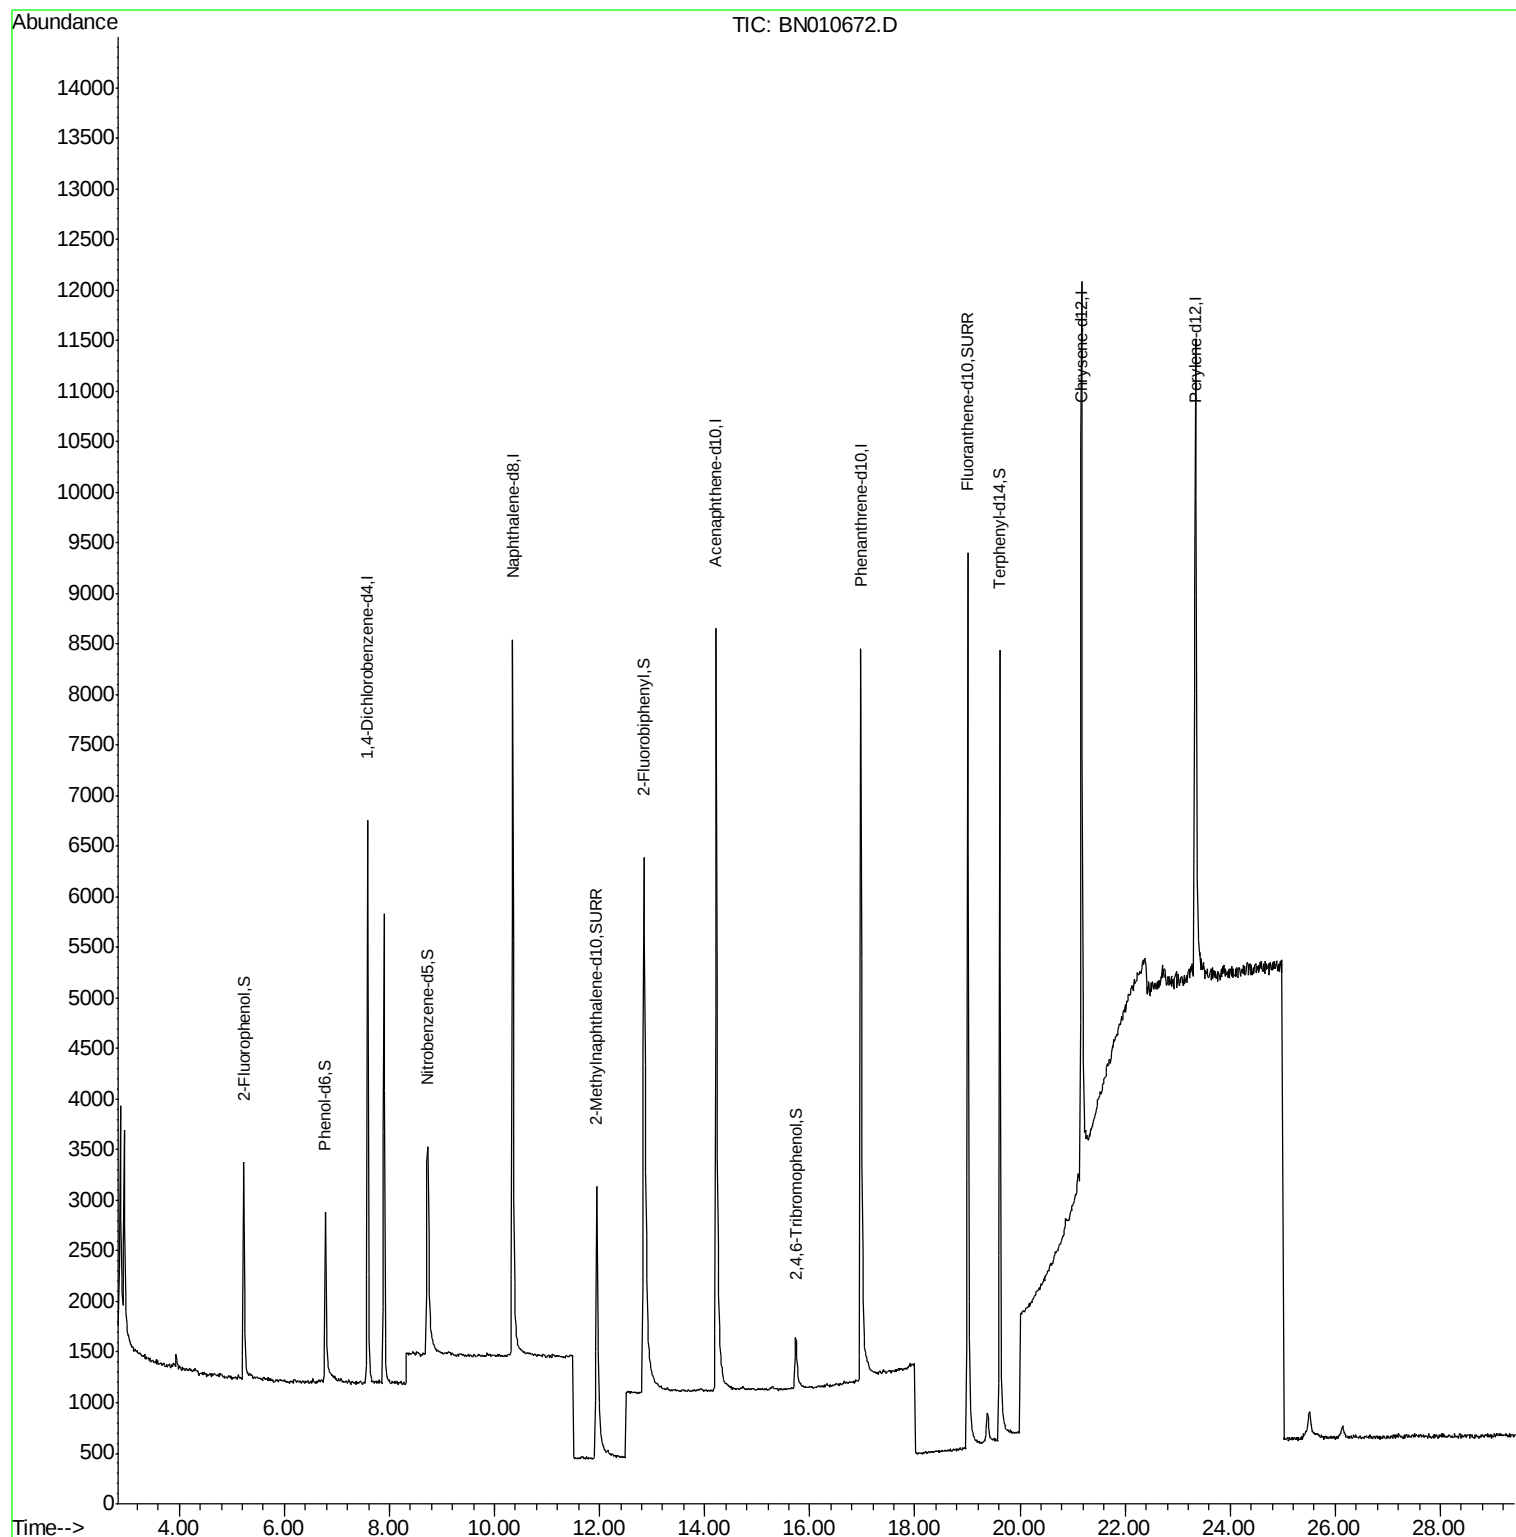


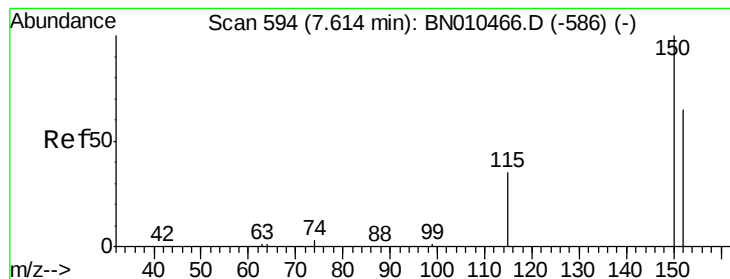




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.58 min Scan# 590
 Delta R.T. -0.00 min
 Lab File: BN010672.D
 Acq: 30 Apr 2020 13:50

Instrument :
 BNA_N
 ClientSampleId :
 PB128575BL

Tot Ion:152 Resp: 3023
 Ion Ratio Lower Upper
 152 100
 150 156.1 121.8 182.6
 115 61.9 45.5 68.3

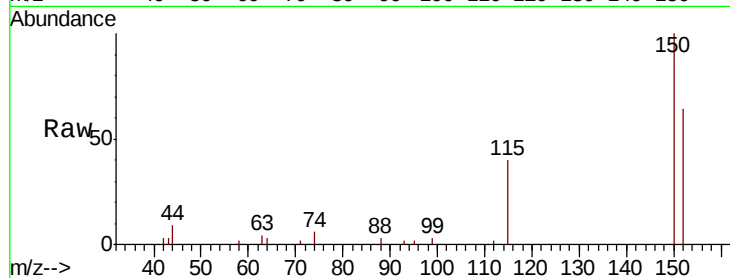


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

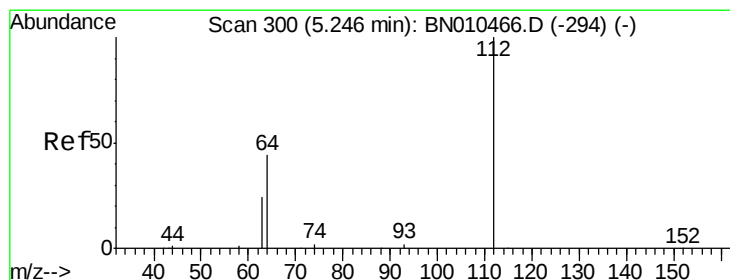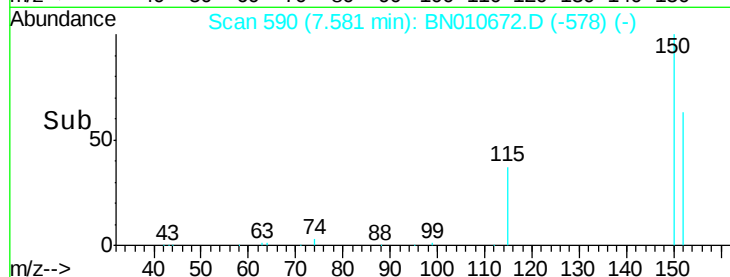
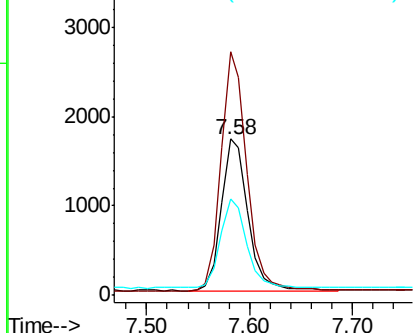



#4
 2-Fluorophenol
 Concen: 0.361 ng
 RT: 5.23 min Scan# 298
 Delta R.T. -0.00 min
 Lab File: BN010672.D
 Acq: 30 Apr 2020 13:50

Tgt Ion:112 Resp: 2389
 Ion Ratio Lower Upper
 112 100
 64 45.1 35.8 53.8
 63 24.4 19.9 29.9

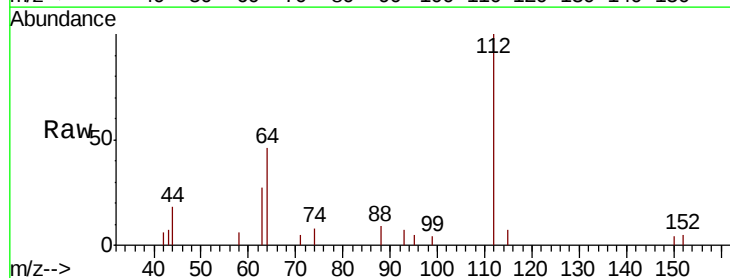

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BNC
 Ion 63.00 (62.70 to 63.70): BNC

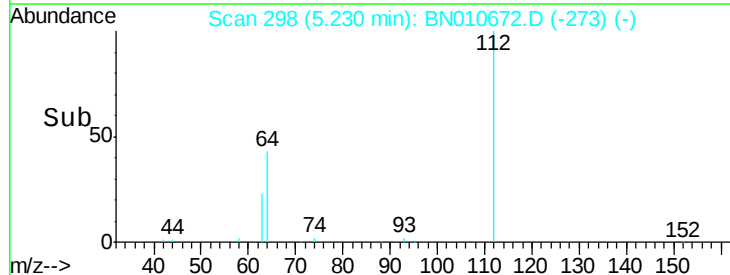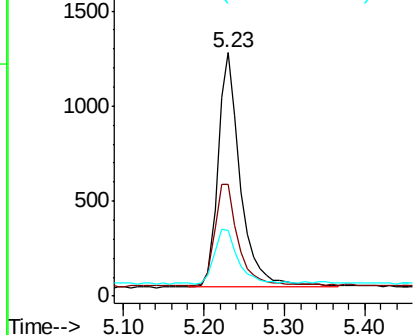



#5

Phenol-d6

Concen: 0.310 ng

RT: 6.78 min Scan# 491

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Instrument :

BNA_N

ClientSampleId :

PB128575BL


Tot Ion: 99 Resp: 2685

Ion Ratio Lower Upper

99 100

42 11.5 9.8 14.6


71 34.3 27.8 41.8

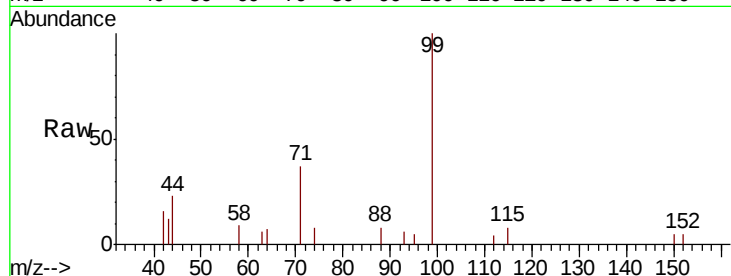



Abundance Ion 99.00 (98.70 to 99.70): BN010466.D (-486) (-)

Ion 42.00 (41.70 to 42.70): BN010466.D (-486) (-)

Ion 71.00 (70.70 to 71.70): BN010466.D (-486) (-)

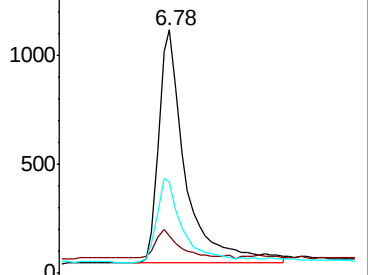

Time-->

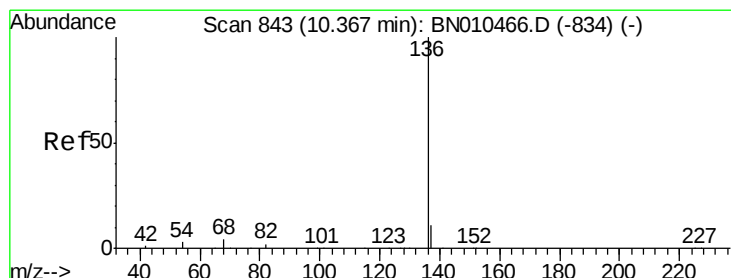

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.34 min Scan# 841

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Tgt Ion: 136 Resp: 12115


Ion Ratio Lower Upper

136 100

137 11.9 8.9 13.3

54 4.4 2.6 4.0#

68 5.1 3.4 5.2

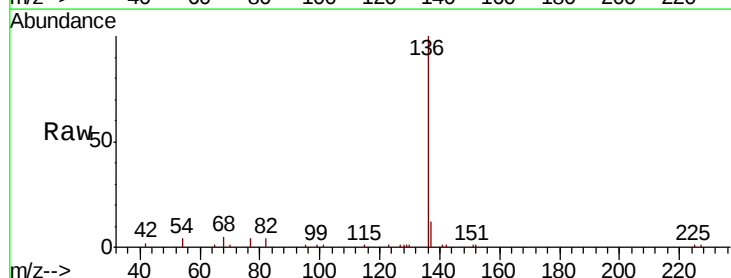


Abundance Ion 136.00 (135.70 to 136.70): BN010466.D (-834) (-)


Ion 137.00 (136.70 to 137.70): BN010466.D (-834) (-)


Ion 54.00 (53.70 to 54.70): BN010466.D (-834) (-)

Ion 68.00 (67.70 to 68.70): BN010466.D (-834) (-)

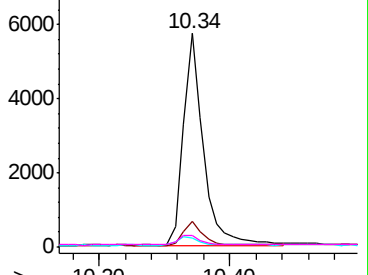

Time-->





#8

Nitrobenzene-d5

Concen: 0.357 ng

RT: 8.73 min Scan# 714

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Instrument :

BNA_N

ClientSampleId :

PB128575BL


Tot Ion: 82 Resp: 3020

Ion Ratio Lower Upper

82 100

128 49.2 41.3 61.9

54 31.5 23.4 35.0

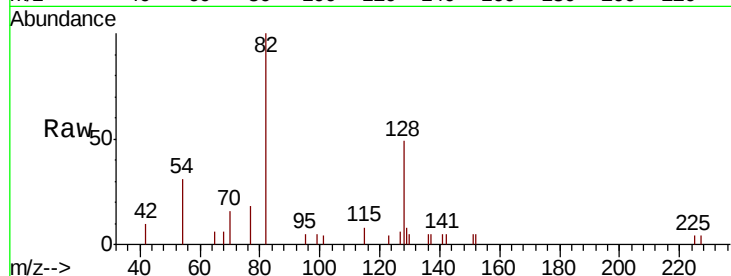


Abundance Ion 82.00 (81.70 to 82.70): BN010466.D (-711) (-)

Ion 128.00 (127.70 to 128.70): BN010466.D (-711) (-)

Ion 54.00 (53.70 to 54.70): BN010466.D (-711) (-)

Time-->




Abundance Ion 82.00 (81.70 to 82.70): BN010672.D (-705) (-)

Ion 128.00 (127.70 to 128.70): BN010672.D (-705) (-)

Ion 54.00 (53.70 to 54.70): BN010672.D (-705) (-)

Time-->

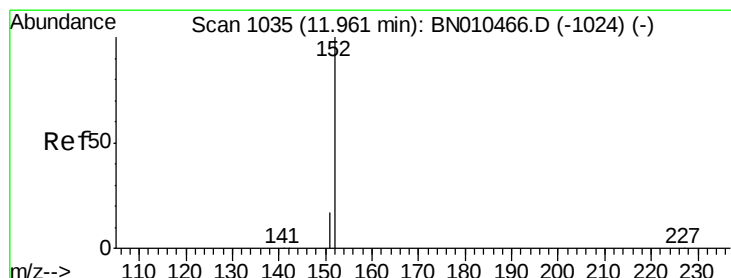

#11

2-Methylnaphthalene-d10

Concen: 0.351 ng

RT: 11.94 min Scan# 1031

Delta R.T. 0.01 min

Lab File: BN010672.D


Acq: 30 Apr 2020 13:50

Tgt Ion: 152 Resp: 7000

Ion Ratio Lower Upper

152 100


151 18.6 15.3 22.9

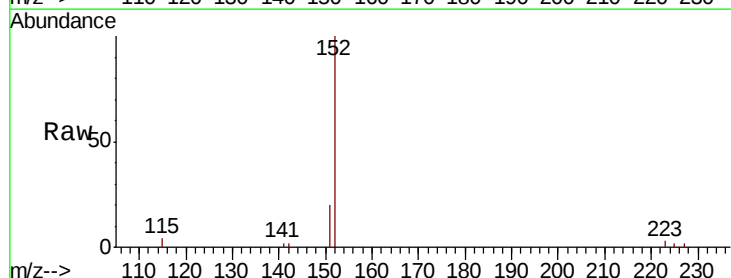

Abundance Ion 152.00 (151.70 to 152.70): BN010466.D (-1024) (-)

Ion 151.00 (150.70 to 151.70): BN010466.D (-1024) (-)


Time-->



Abundance Ion 152.00 (151.70 to 152.70): BN010672.D (-983) (-)

Ion 151.00 (150.70 to 151.70): BN010672.D (-983) (-)

Time-->

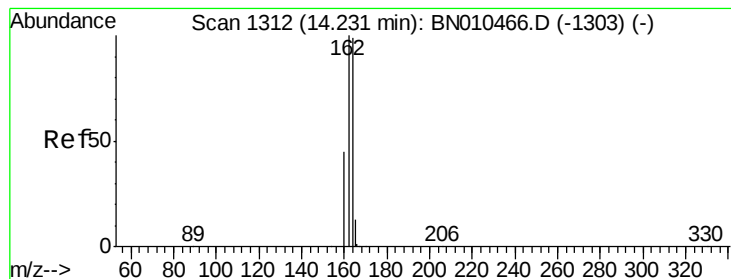

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.21 min Scan# 1311

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Instrument :

BNA_N

ClientSampleId :

PB128575BL


Tot Ion:164 Resp: 7490

Ion Ratio Lower Upper

164 100

162 102.8 80.6 121.0




160 48.7 36.5 54.7

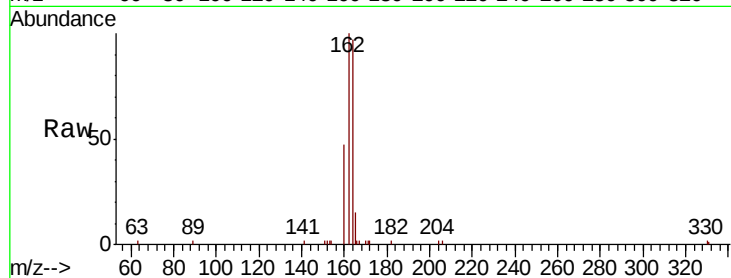

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

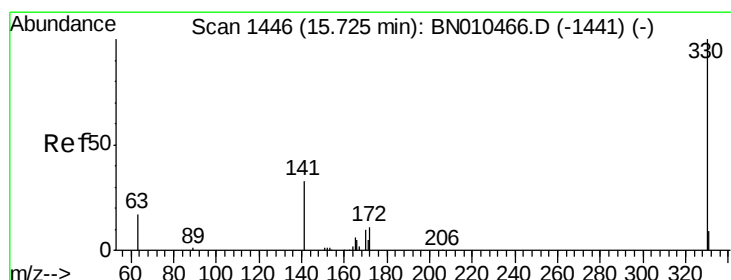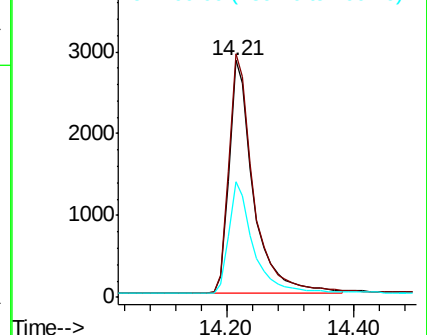

#14

2,4,6-Tribromophenol

Concen: 0.222 ng

RT: 15.74 min Scan# 1448

Delta R.T. 0.03 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50


Tgt Ion:330 Resp: 784

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 36.2 28.1 42.1

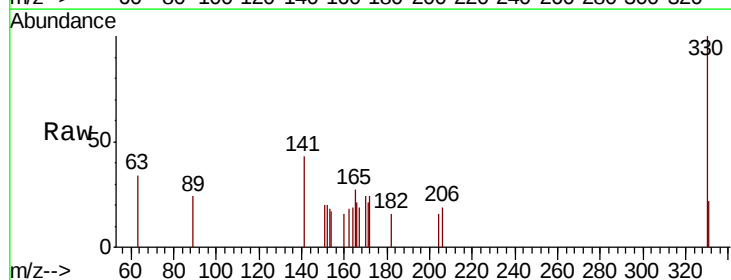


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




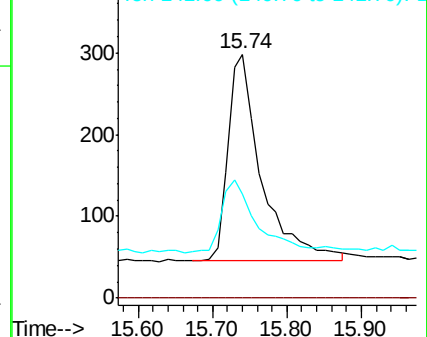




#15
2-Fluorobiphenyl
Concen: 0.346 ng
RT: 12.84 min Scan# 1188
Delta R.T. 0.02 min
Lab File: BN010672.D
Acq: 30 Apr 2020 13:50




Instrument :
BNA_N
ClientSampleId :
PB128575BL


Tot Ion:172 Resp: 9431
Ion Ratio Lower Upper
172 100
171 35.7 28.2 42.2
170 23.9 18.4 27.6

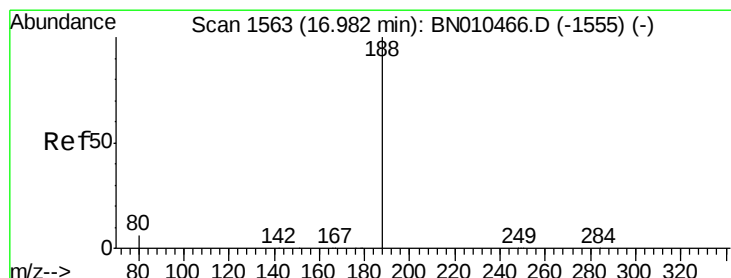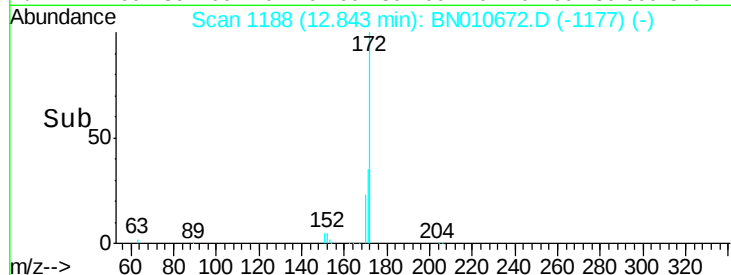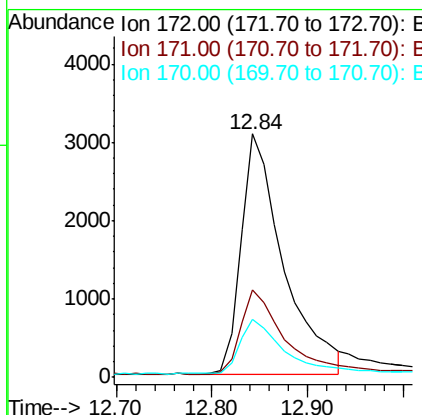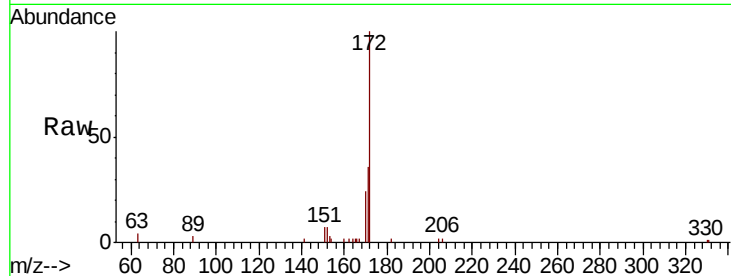

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 16.97 min Scan# 1563
Delta R.T. 0.02 min
Lab File: BN010672.D
Acq: 30 Apr 2020 13:50

Tgt Ion:188 Resp: 16324
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.6 5.0 7.6#

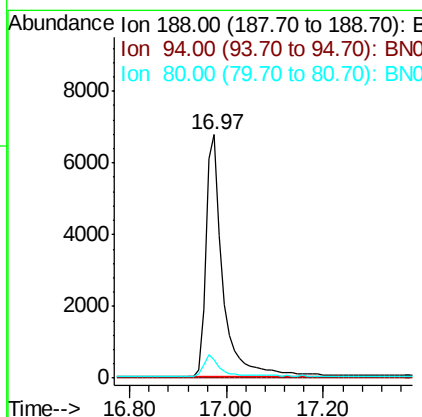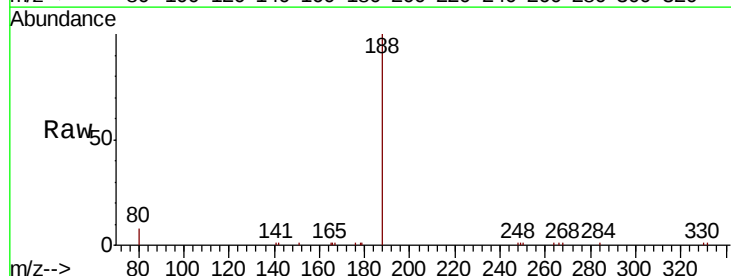

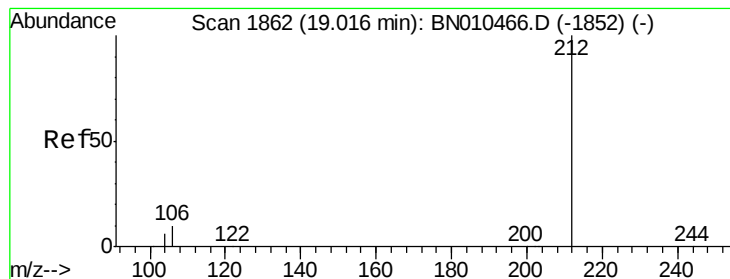

#25

Fluoranthene-d10

Concen: 0.291 ng

RT: 19.00 min Scan# 1861

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Instrument :

BNA_N

ClientSampleId :

PB128575BL


Tot Ion:212 Resp: 14414

Ion Ratio Lower Upper

212 100

106 10.0 7.8 11.6




104 5.5 4.5 6.7

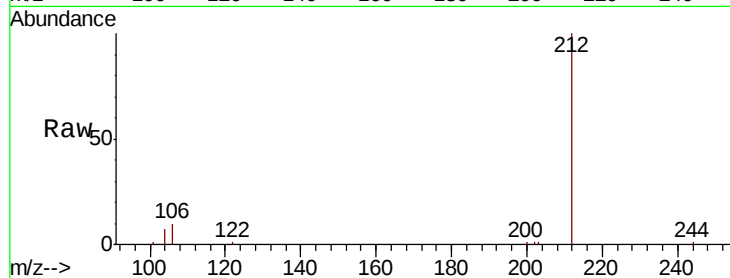

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

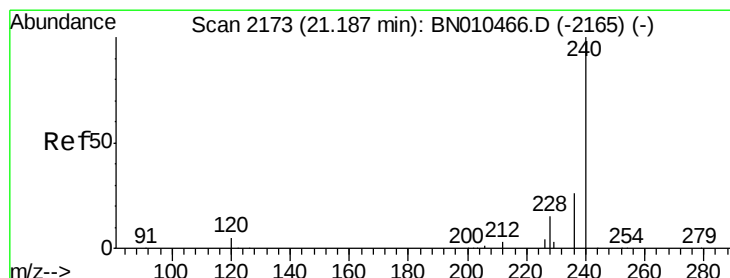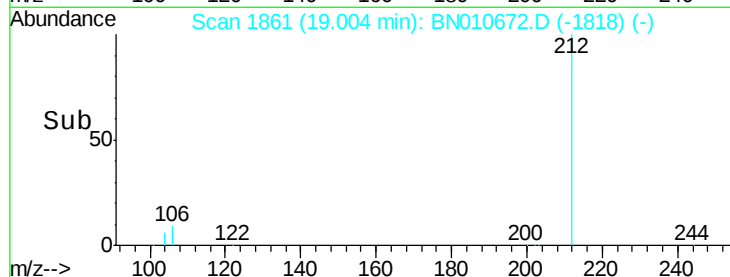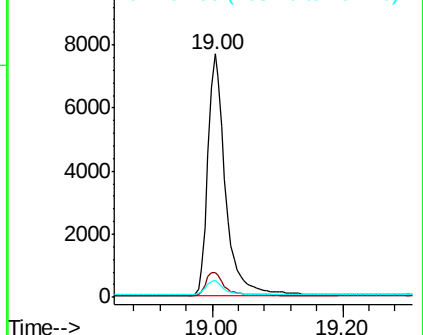

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.17 min Scan# 2173

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50


Tgt Ion:240 Resp: 11647

Ion Ratio Lower Upper

240 100

120 8.8 4.8 7.2#



236 27.3 21.4 32.0

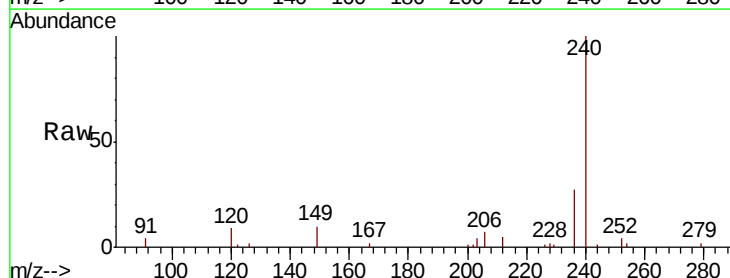


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

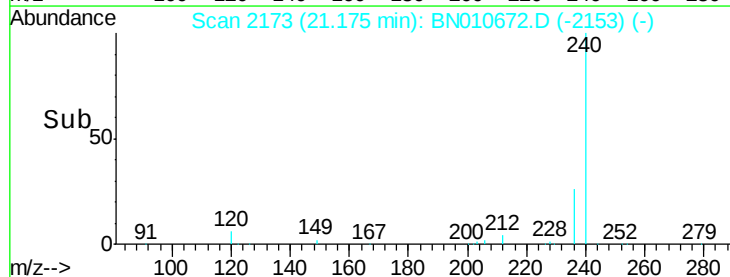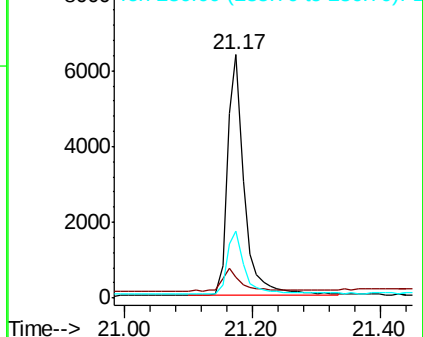

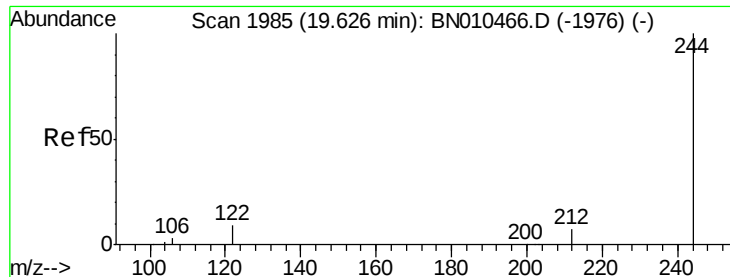

#29

Terphenyl-d14

Concen: 0.404 ng

RT: 19.61 min Scan# 1984

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50

Instrument :

BNA_N

ClientSampleId :

PB128575BL


Tot Ion:244 Resp: 10768

Ion Ratio Lower Upper

244 100

212 8.7 6.2 9.4

122 10.2 7.8 11.8

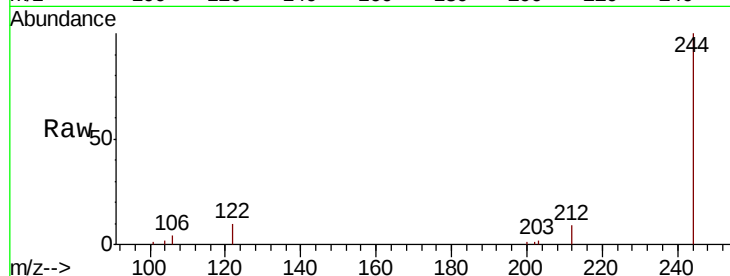


Abundance Ion 244.00 (243.70 to 244.70): E


Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

Time-->

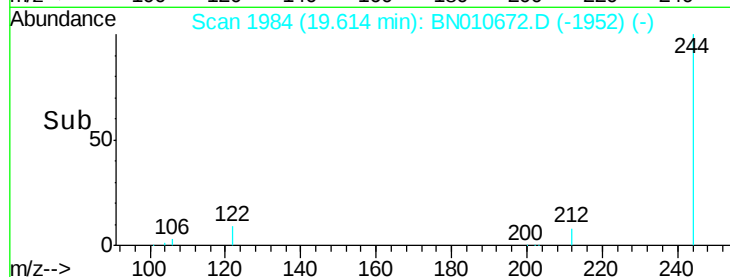

Time-->

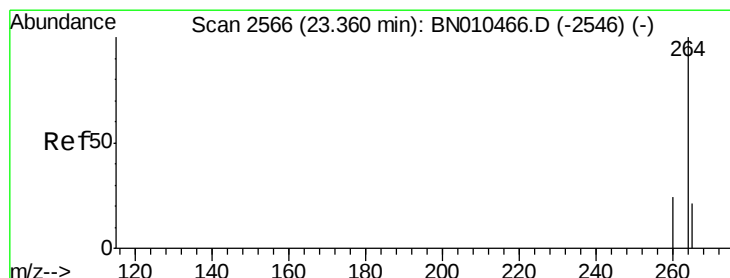

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.34 min Scan# 2561

Delta R.T. 0.01 min

Lab File: BN010672.D

Acq: 30 Apr 2020 13:50


Tgt Ion:264 Resp: 10496

Ion Ratio Lower Upper

264 100

260 25.0 19.8 29.8

265 98.2 42.3 63.5#

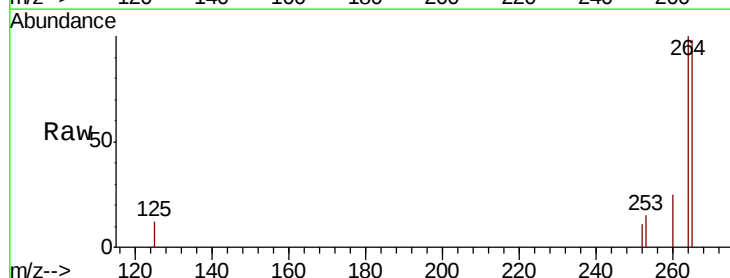


Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

Time-->

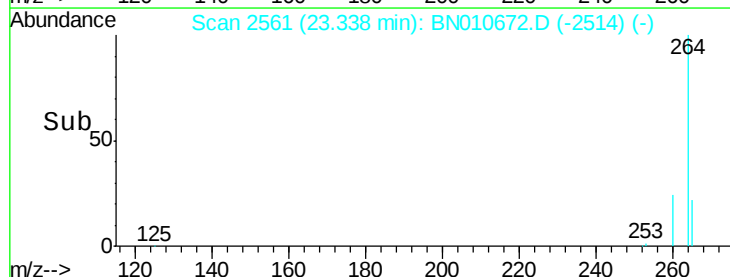

Time-->