


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN043020\
 Data File : BN010667.D
 Acq On : 30 Apr 2020 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN041320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 11:18:31 2020

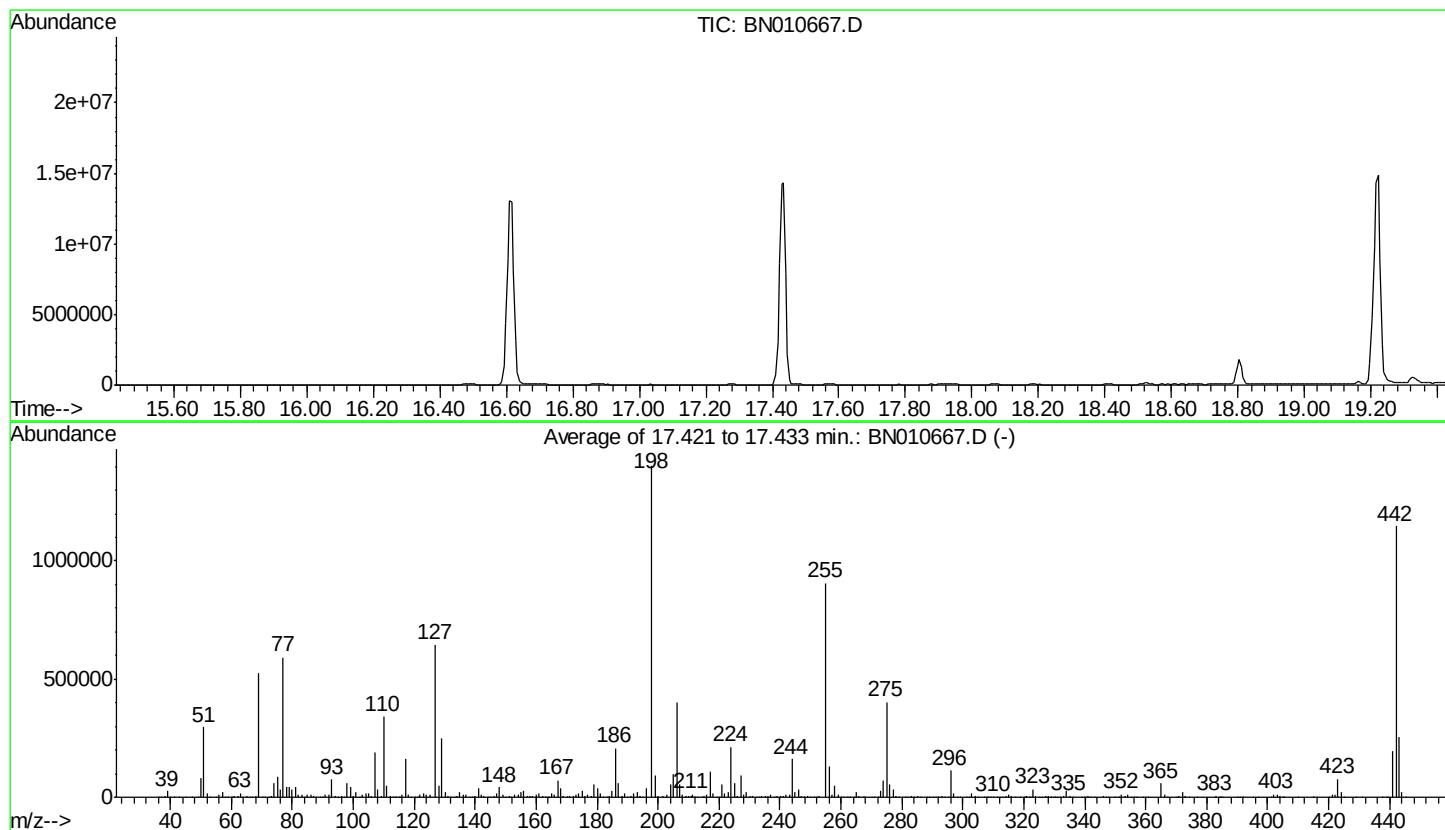

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	296490	PASS
68	69	0.00	2	1.2	6343	PASS
69	198	0.00	100	37.4	525120	PASS
70	69	0.00	2	0.5	2682	PASS
127	198	10	80	46.1	647061	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1403733	PASS
199	198	5	9	6.6	92578	PASS
275	198	10	60	28.6	401898	PASS
365	198	1	100	4.1	58240	PASS
441	198	0.01	100	13.7	192768	PASS
442	198	50	100	81.8	1148522	PASS
443	442	15	24	22.0	253200	PASS