




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031338.D
 Acq On : 01 May 2024 03:49
 Operator : MA/JU
 Sample : P2203-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CW8

Manual IntegrationsAPPROVED

Quant Time: May 01 05:27:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

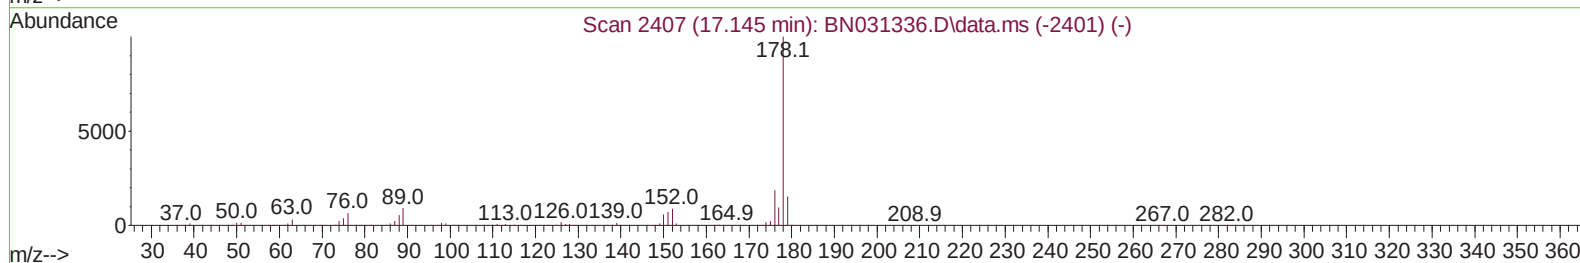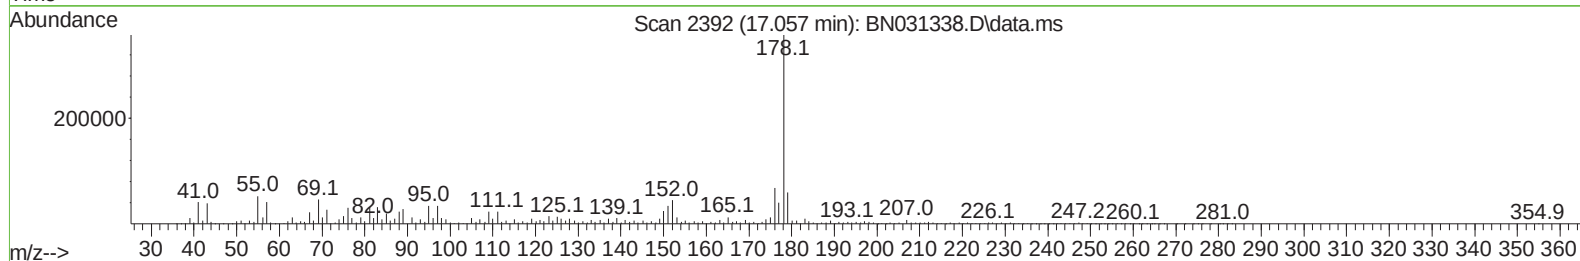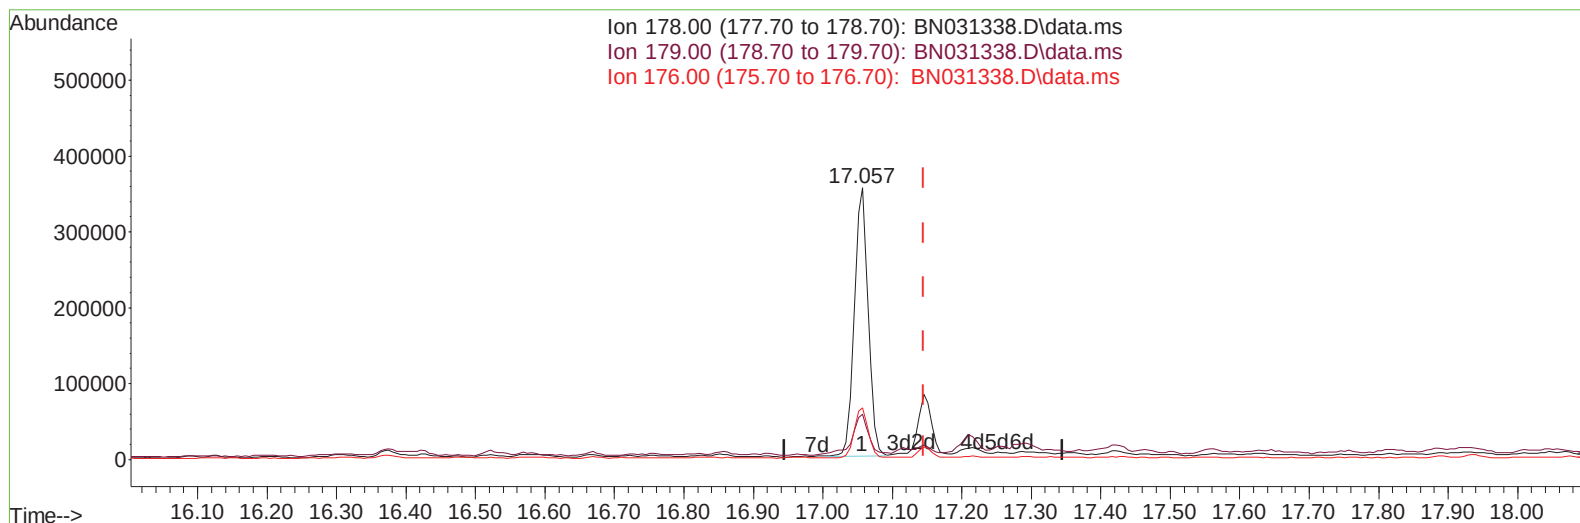

TIC: BN031338.D\data.ms

(74) Anthracene

17.057min (-0.088) 8.38 ng/ul

response 488902

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.00	16.55
176.00	18.90	19.08
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031338.D
 Acq On : 01 May 2024 03:49
 Operator : MA/JU
 Sample : P2203-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CW8

Manual IntegrationsAPPROVED

Quant Time: May 01 05:27:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

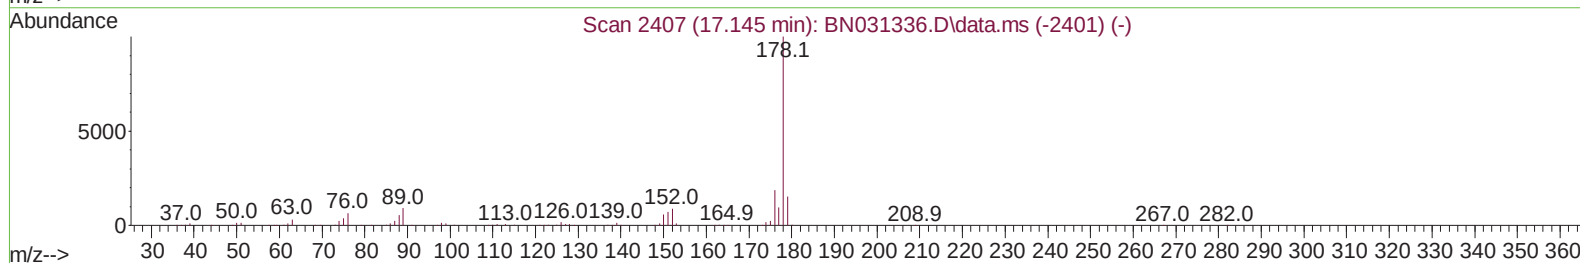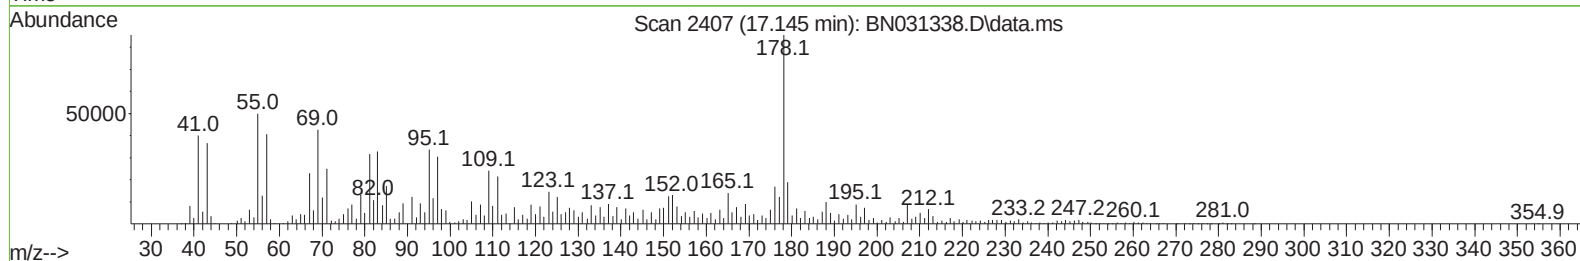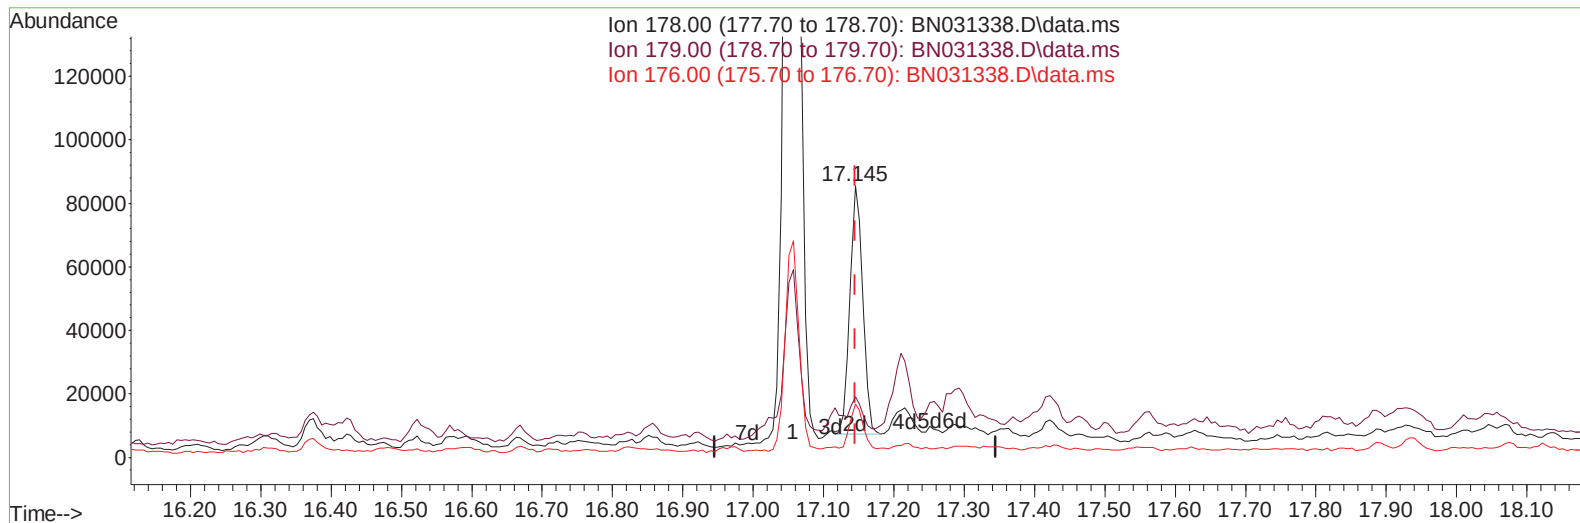

TIC: BN031338.D\data.ms

(74) Anthracene

17.145min (0.000) 1.70 ng/ul m

response 99193

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.00	22.23#
176.00	18.90	19.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031338.D
 Acq On : 01 May 2024 03:49
 Operator : MA/JU
 Sample : P2203-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CW8

Manual IntegrationsAPPROVED

Quant Time: May 01 05:27:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

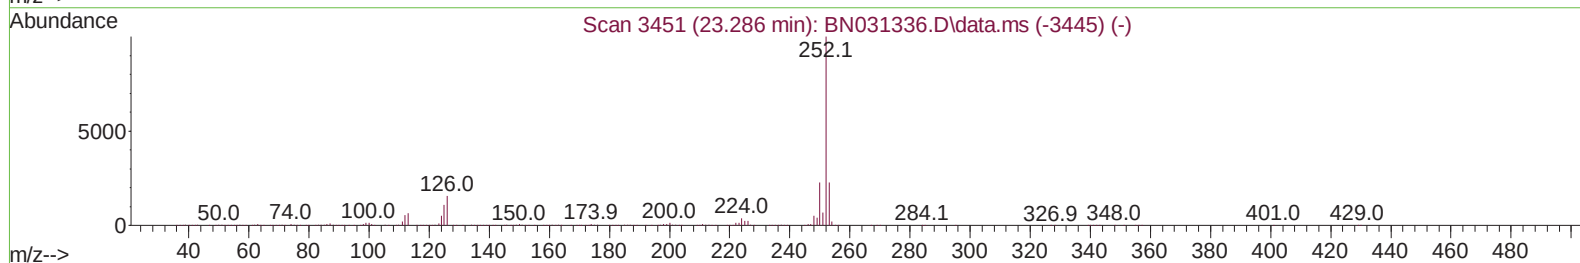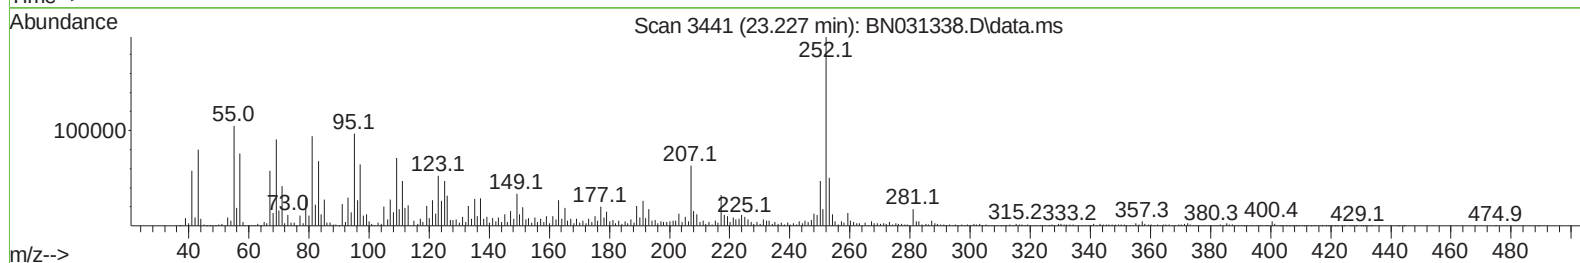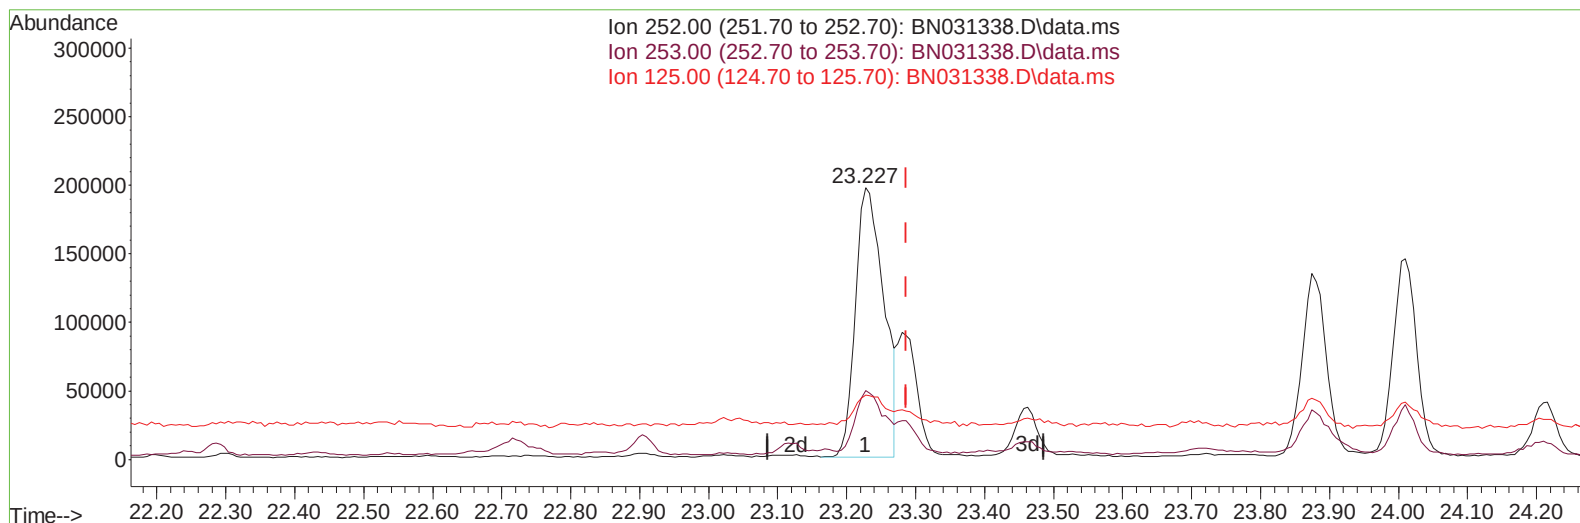

TIC: BN031338.D\data.ms

(91) Benzo(k)fluoranthene

23.227min (-0.059) 11.08 ng/ul

response 560474

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	25.34
125.00	10.90	23.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031338.D
 Acq On : 01 May 2024 03:49
 Operator : MA/JU
 Sample : P2203-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CW8

Manual IntegrationsAPPROVED

Quant Time: May 01 05:27:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

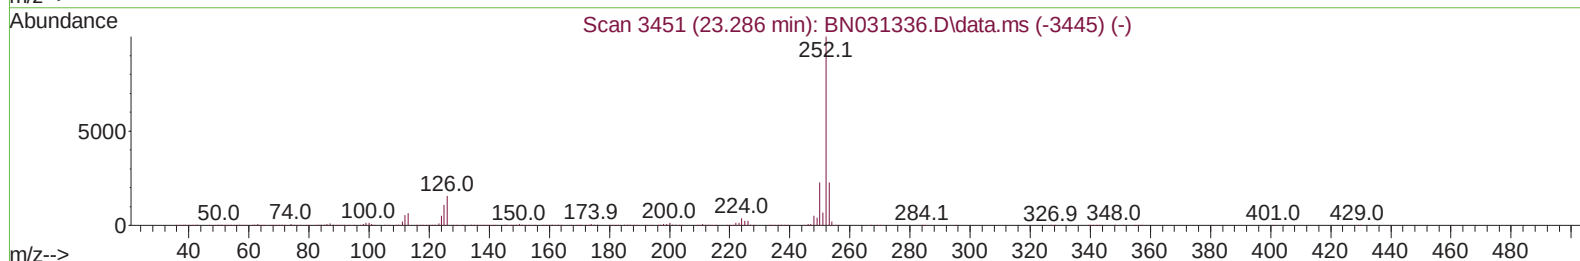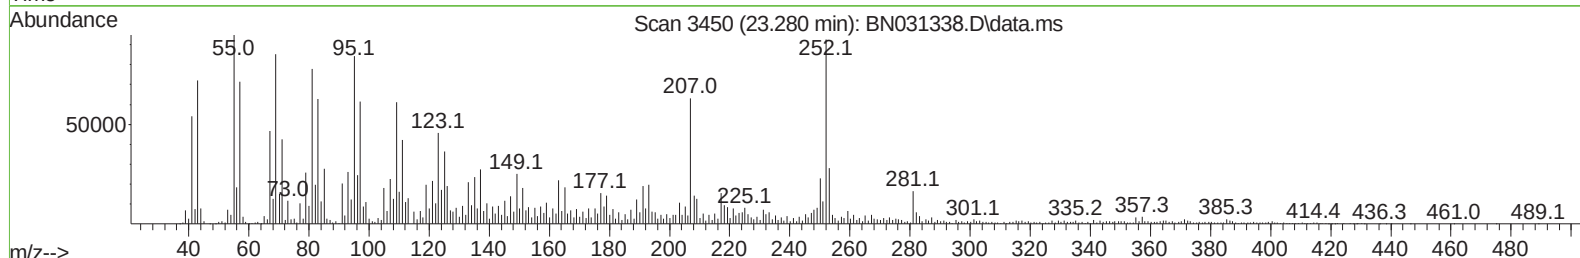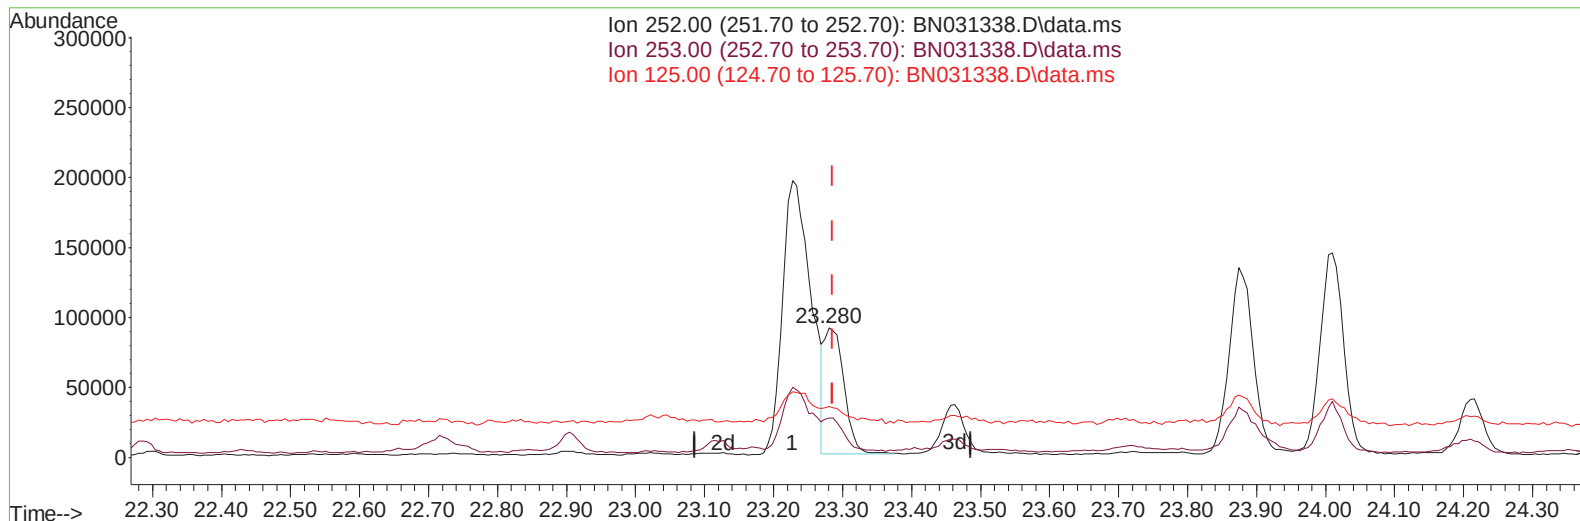

TIC: BN031338.D\data.ms

(91) Benzo(k)fluoranthene

23.280min (-0.006) 3.51 ng/ul m

response 177596

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.30	30.44#
125.00	10.90	39.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031338.D
 Acq On : 01 May 2024 03:49
 Operator : MA/JU
 Sample : P2203-09
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CW8

Manual IntegrationsAPPROVED

Quant Time: May 01 05:30:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

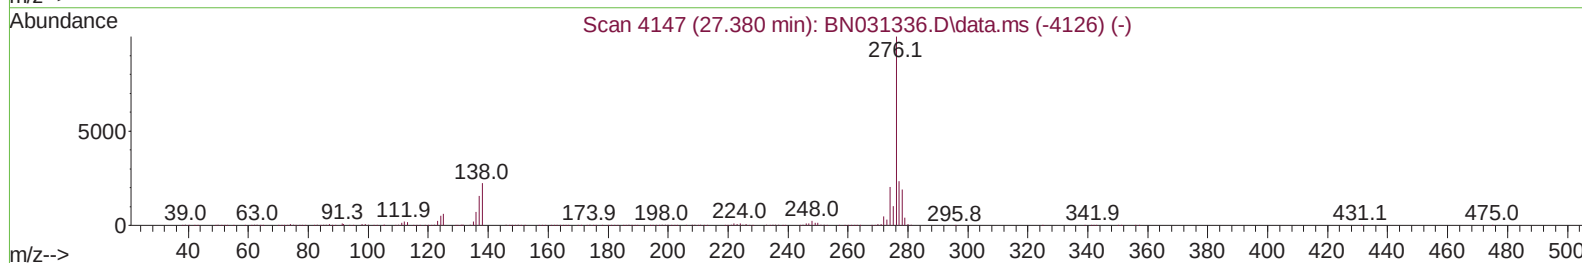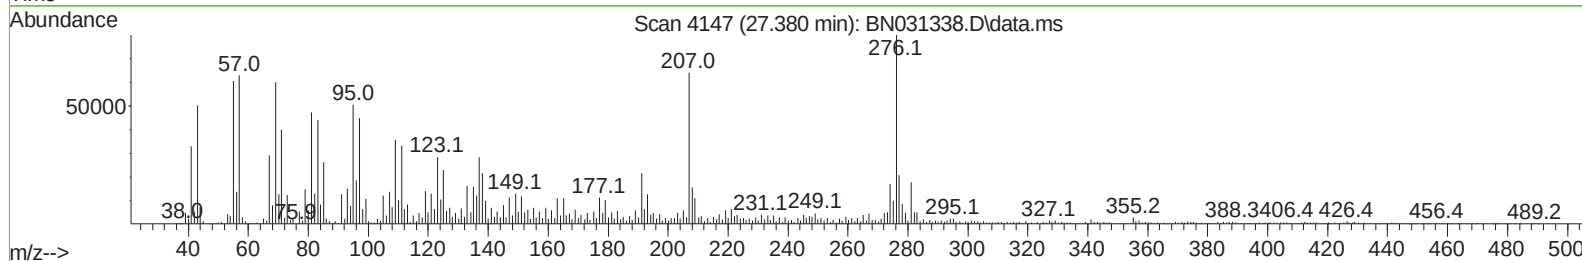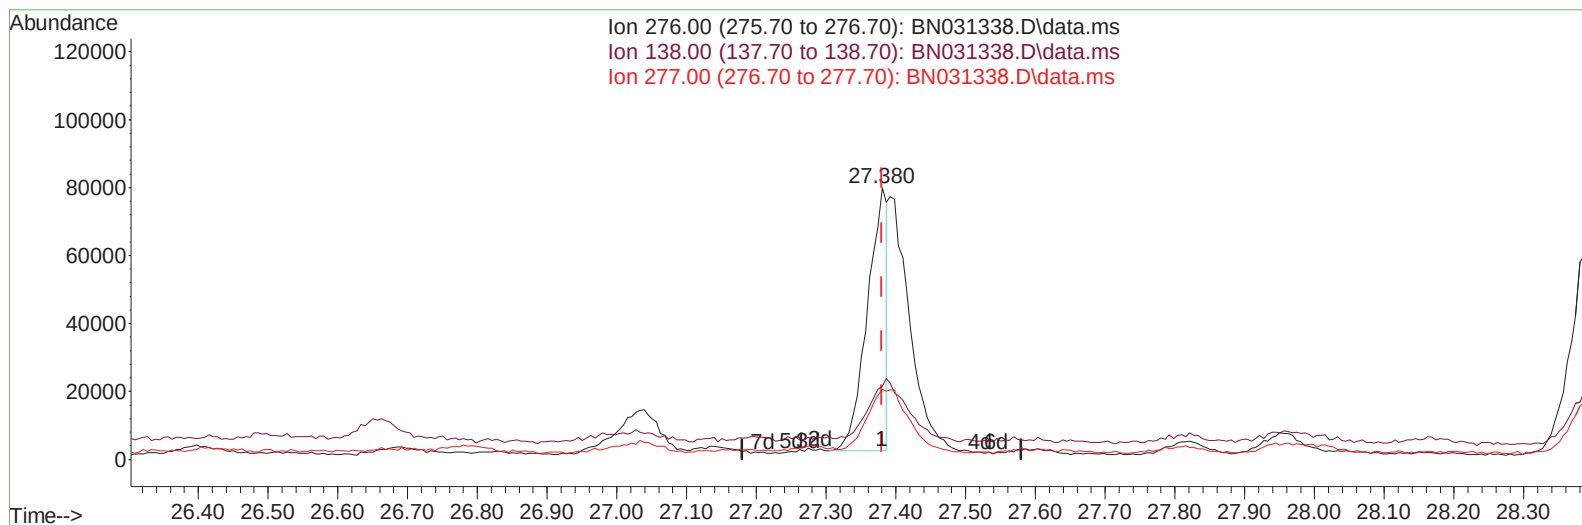

TIC: BN031338.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

27.380min (0.000) 2.90 ng/u1

response 151216

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.60	26.98
277.00	24.40	25.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031338.D
Acq On : 01 May 2024 03:49
Operator : MA/JU
Sample : P2203-09
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CW8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

Quant Time: May 01 05:30:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

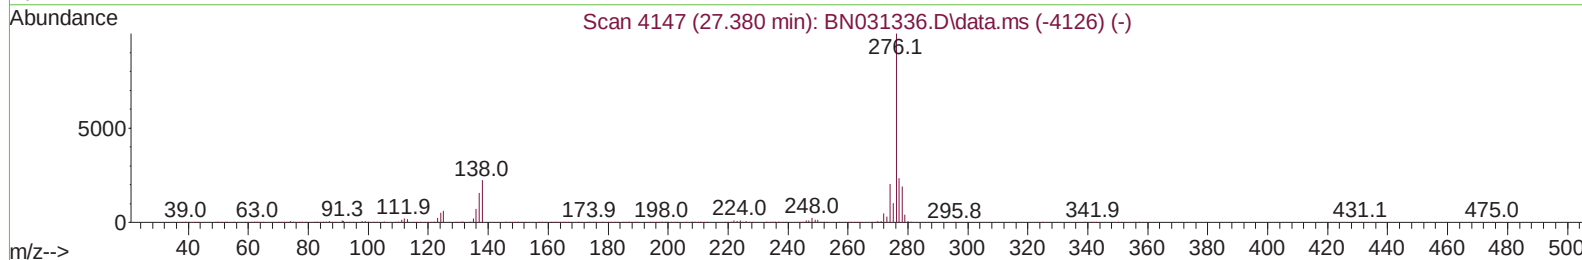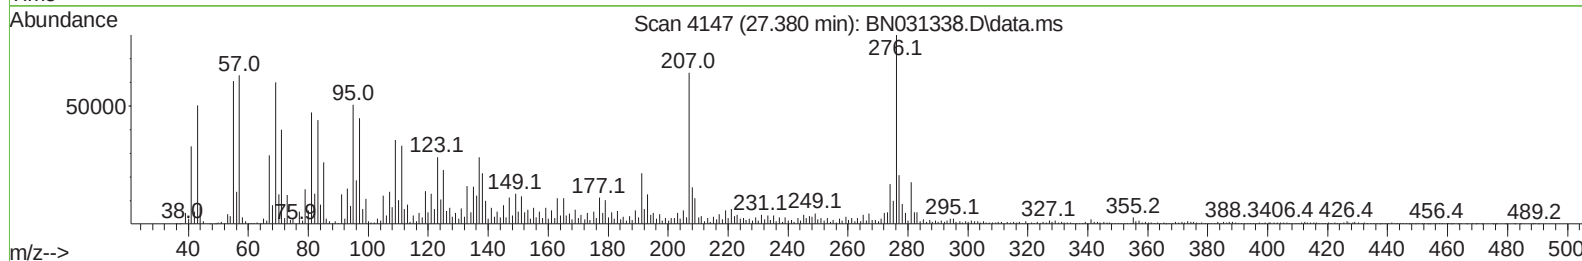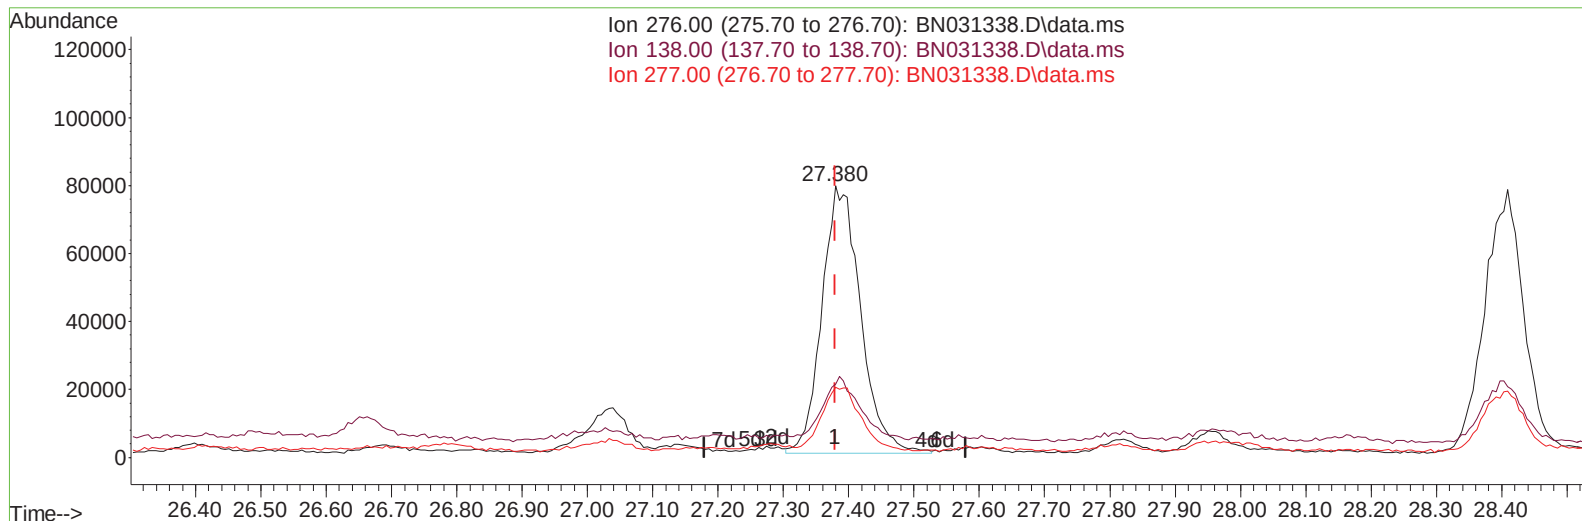

TIC: BN031338.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

27.380min (0.000) 6.21 ng/ul m

response 323666

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	22.60	26.98
277.00	24.40	25.86
0.00	0.00	0.00