

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031339.D
 Acq On : 01 May 2024 04:29
 Operator : MA/JU
 Sample : P2203-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :

BNA_N




ClientSampleId :

E1CY7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

Quant Time: May 01 05:39:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

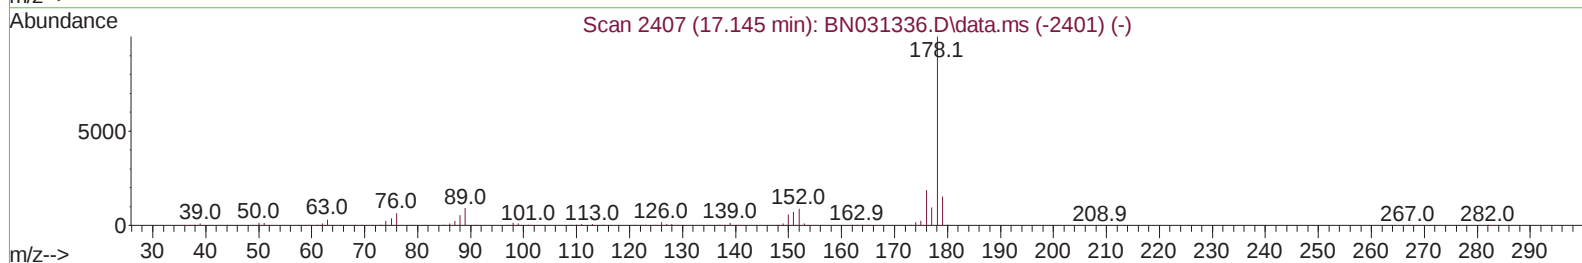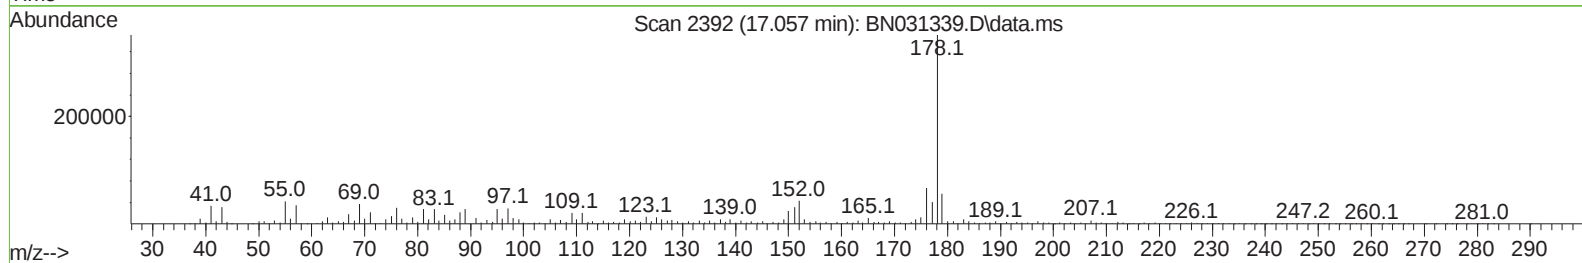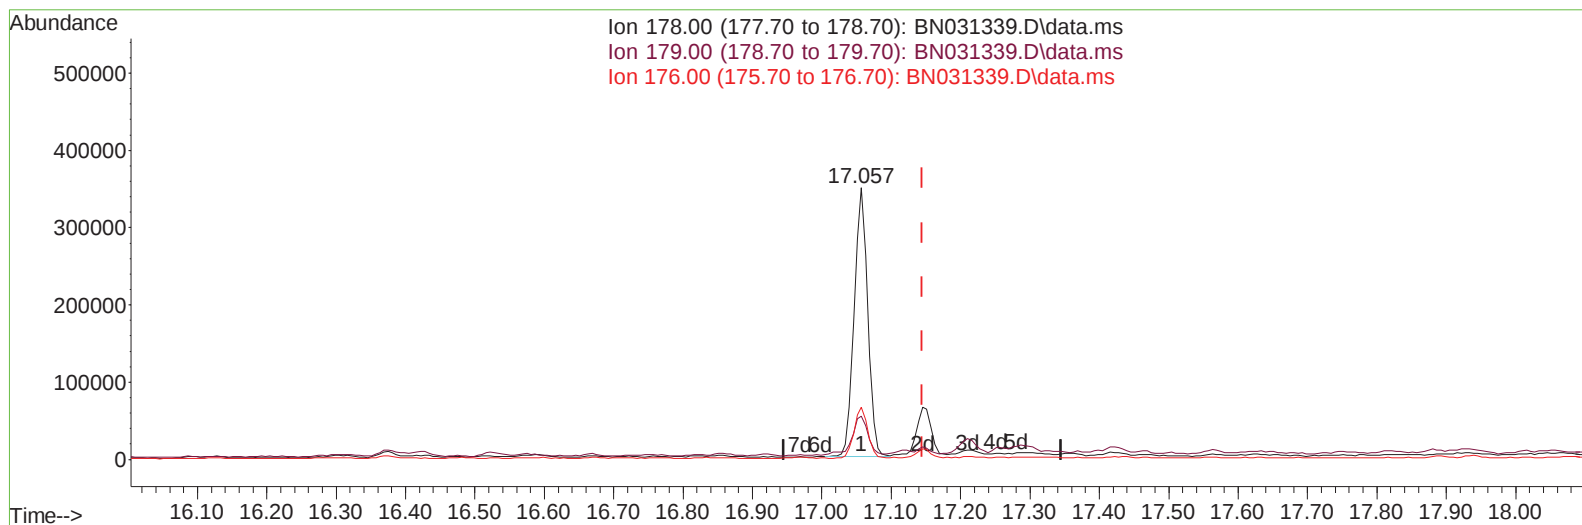

TIC: BN031339.D\data.ms

(74) Anthracene

17.057min (-0.088) 6.14 ng/u1

response 471853

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.00	16.00
176.00	18.90	19.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031339.D
Acq On : 01 May 2024 04:29
Operator : MA/JU
Sample : P2203-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY7

Manual IntegrationsAPPROVED

Quant Time: May 01 05:39:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

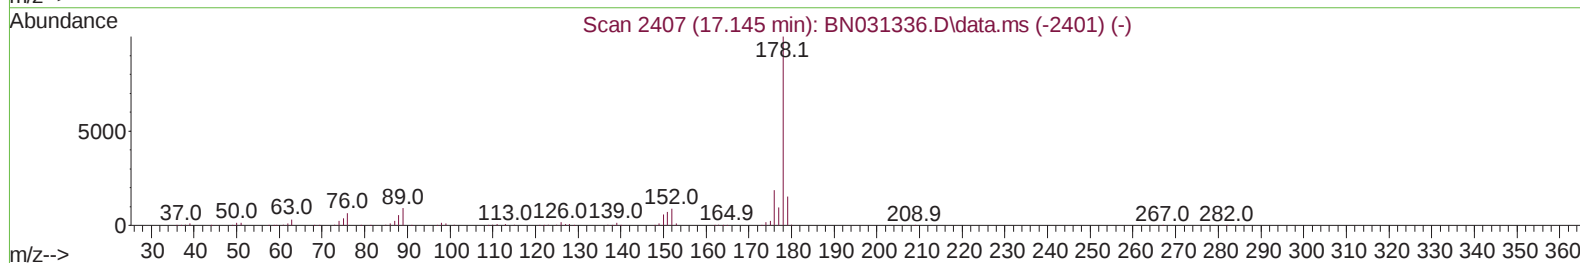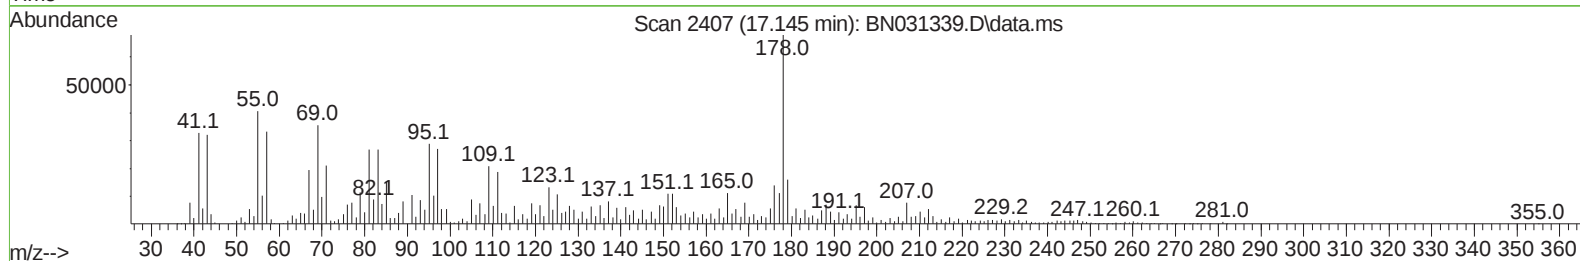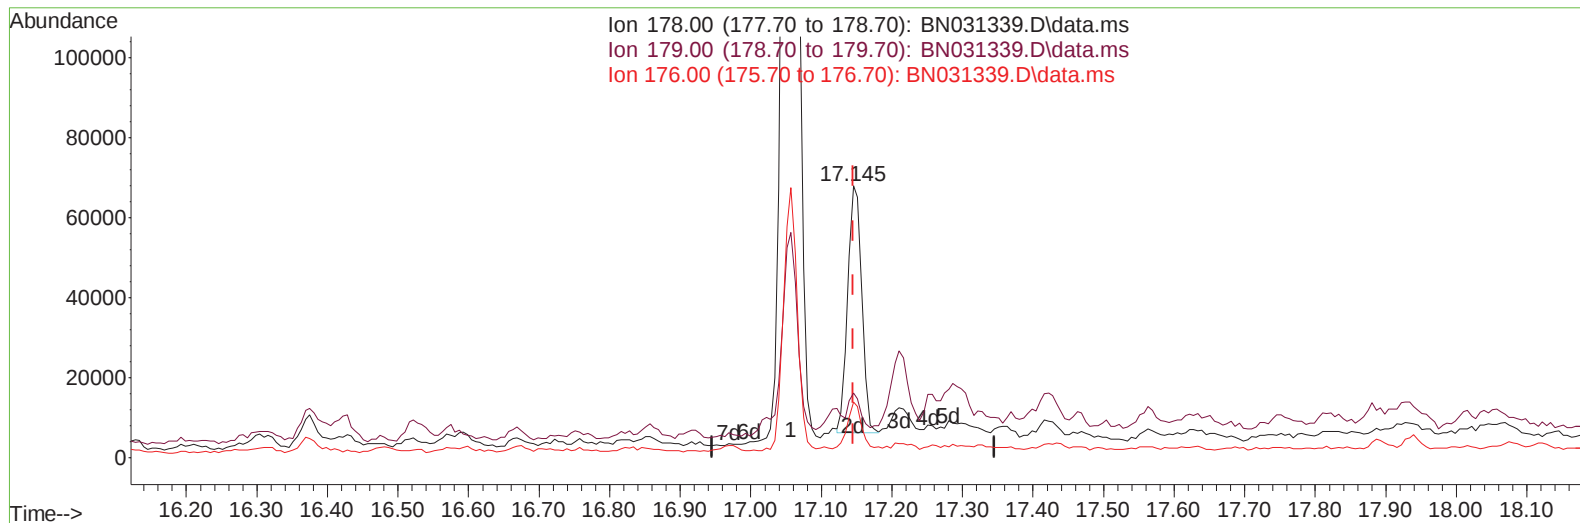

TIC: BN031339.D\data.ms

(74) Anthracene

17.145min (+ 0.000) 1.11 ng/u1 m

response 85295

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.00	23.62#
176.00	18.90	20.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031339.D
Acq On : 01 May 2024 04:29
Operator : MA/JU
Sample : P2203-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY7

Manual IntegrationsAPPROVED

Quant Time: May 01 05:39:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

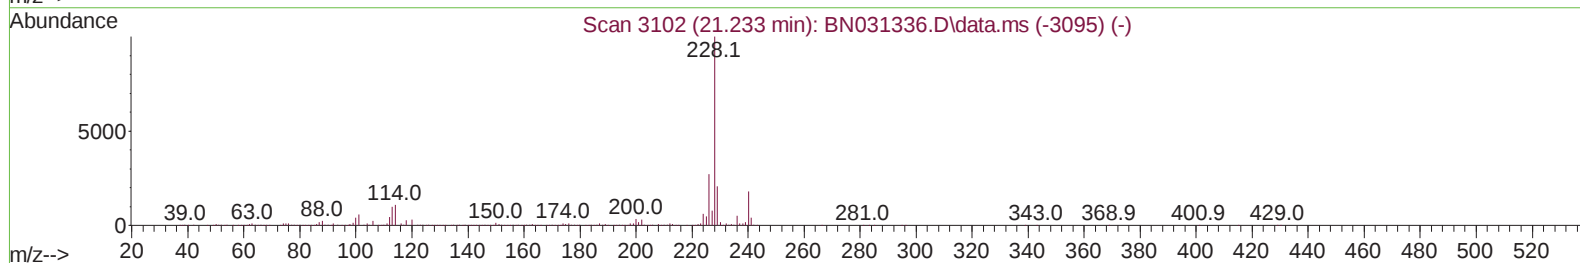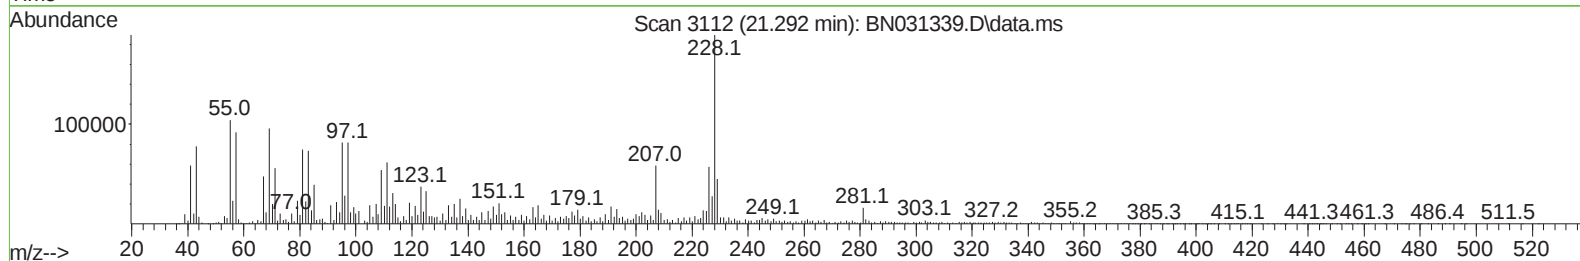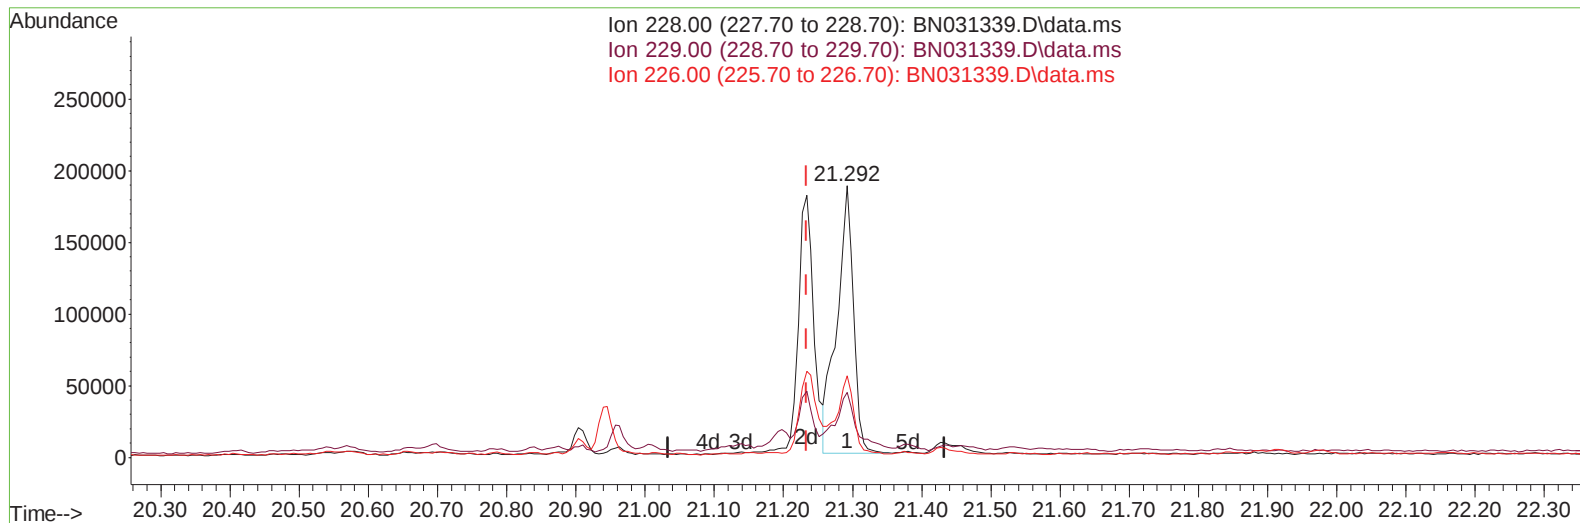

TIC: BN031339.D\data.ms

(85) Benzo(a)anthracene

21.292min (+ 0.059) 4.44 ng/u1

response 310470

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	23.84
226.00	26.40	30.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031339.D
Acq On : 01 May 2024 04:29
Operator : MA/JU
Sample : P2203-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

Quant Time: May 01 05:39:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

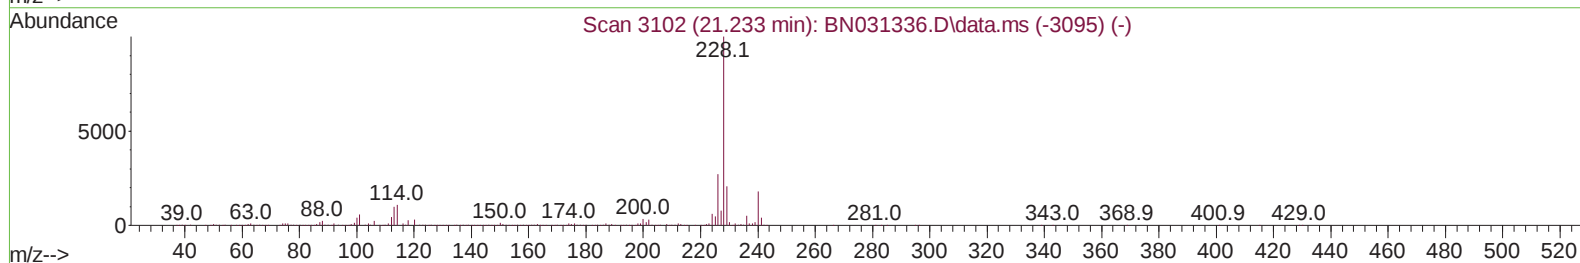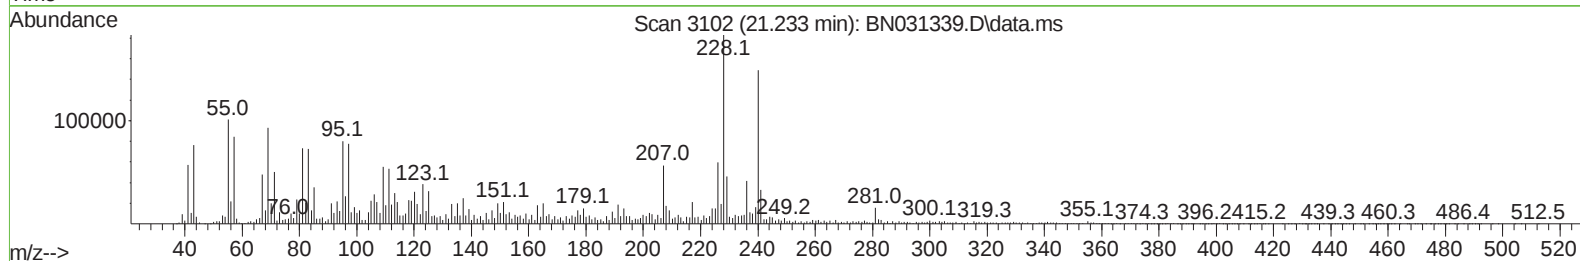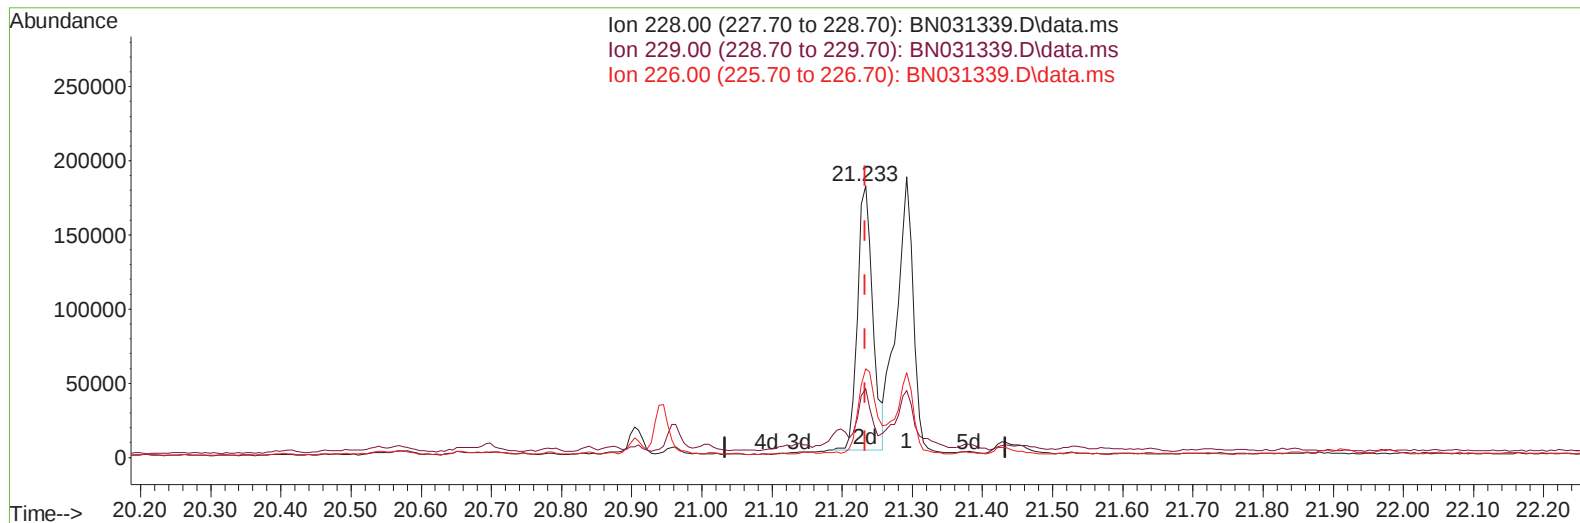

TIC: BN031339.D\data.ms

(85) Benzo(a)anthracene

21.233min (+ 0.000) 3.82 ng/u1 m

response 267339

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.90	25.32#
226.00	26.40	32.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031339.D
Acq On : 01 May 2024 04:29
Operator : MA/JU
Sample : P2203-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CY7

Manual IntegrationsAPPROVED

Quant Time: May 01 05:42:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

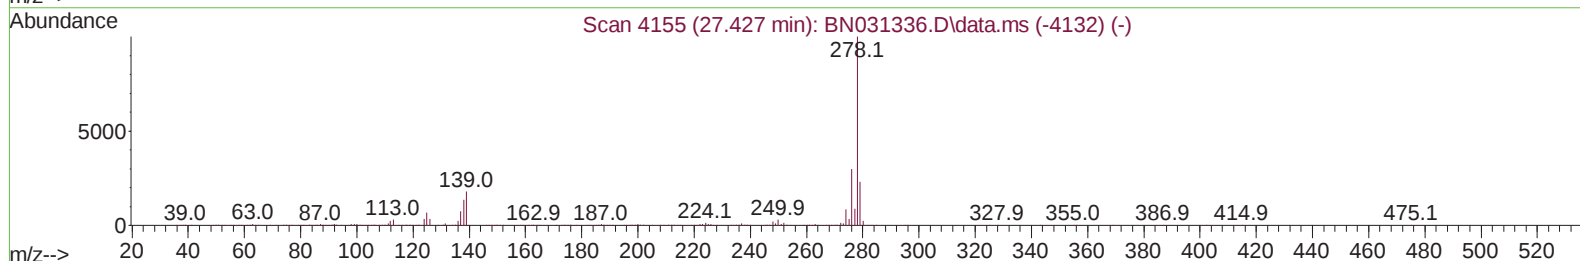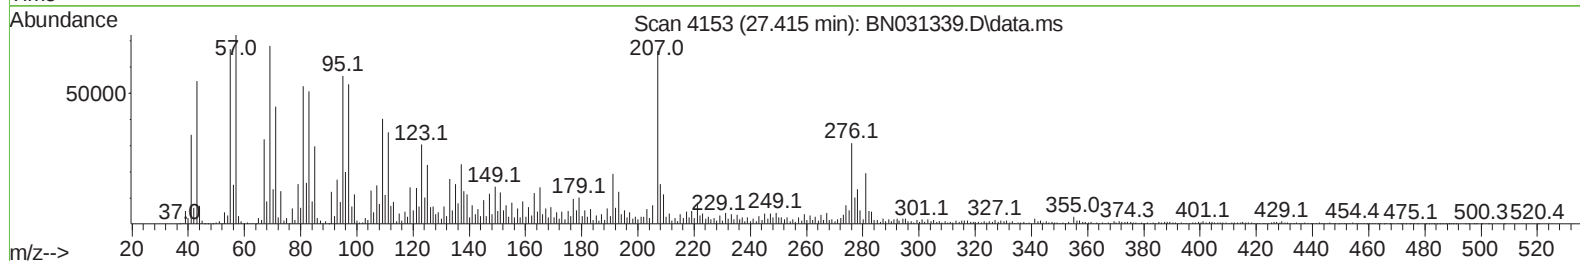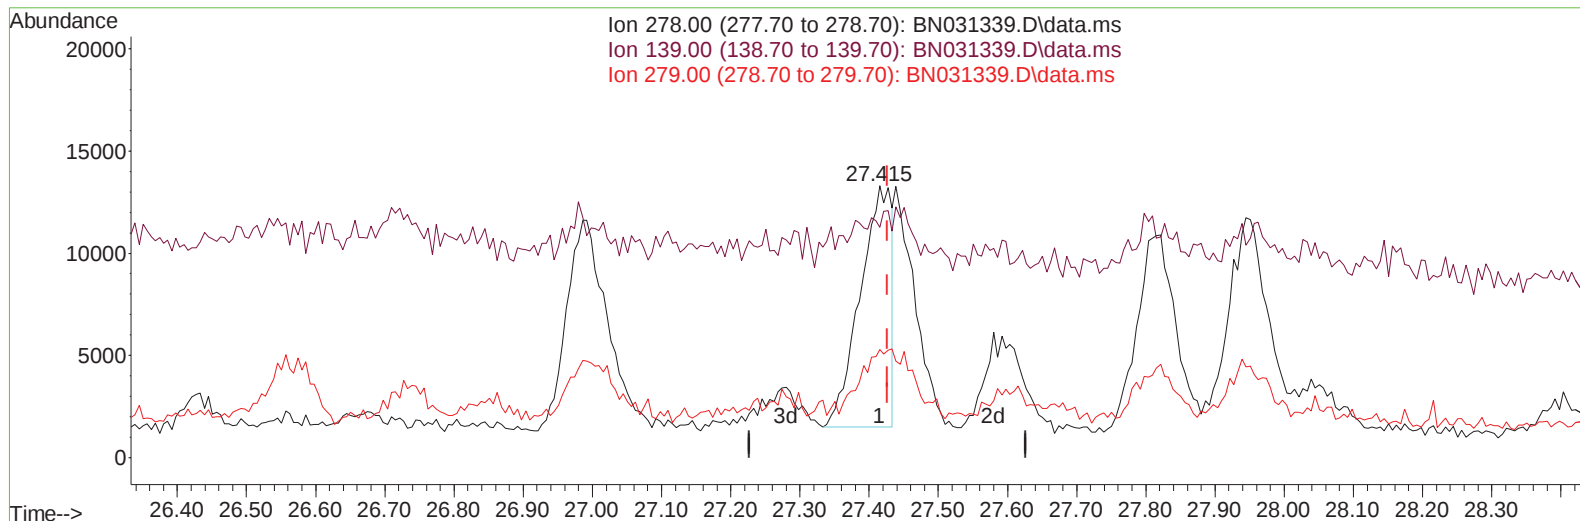

TIC: BN031339.D\data.ms

(95) Dibenzo(a,h)anthracene

27.415min (-0.012) 0.65 ng/u1

response 37365

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	17.40	84.74#
279.00	23.40	39.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031339.D
 Acq On : 01 May 2024 04:29
 Operator : MA/JU
 Sample : P2203-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CY7

Manual IntegrationsAPPROVED

Quant Time: May 01 05:42:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

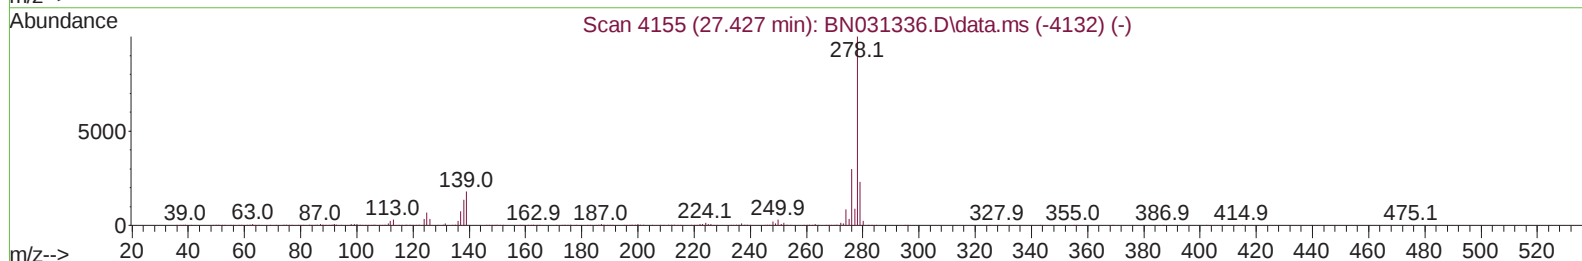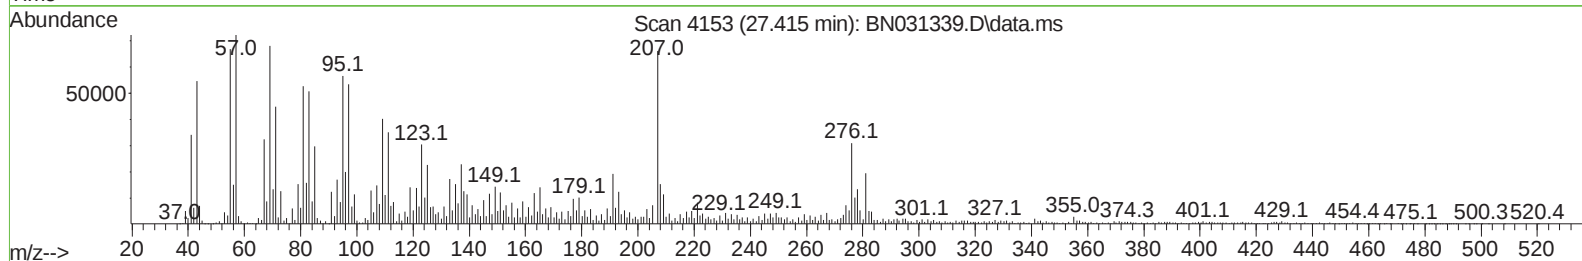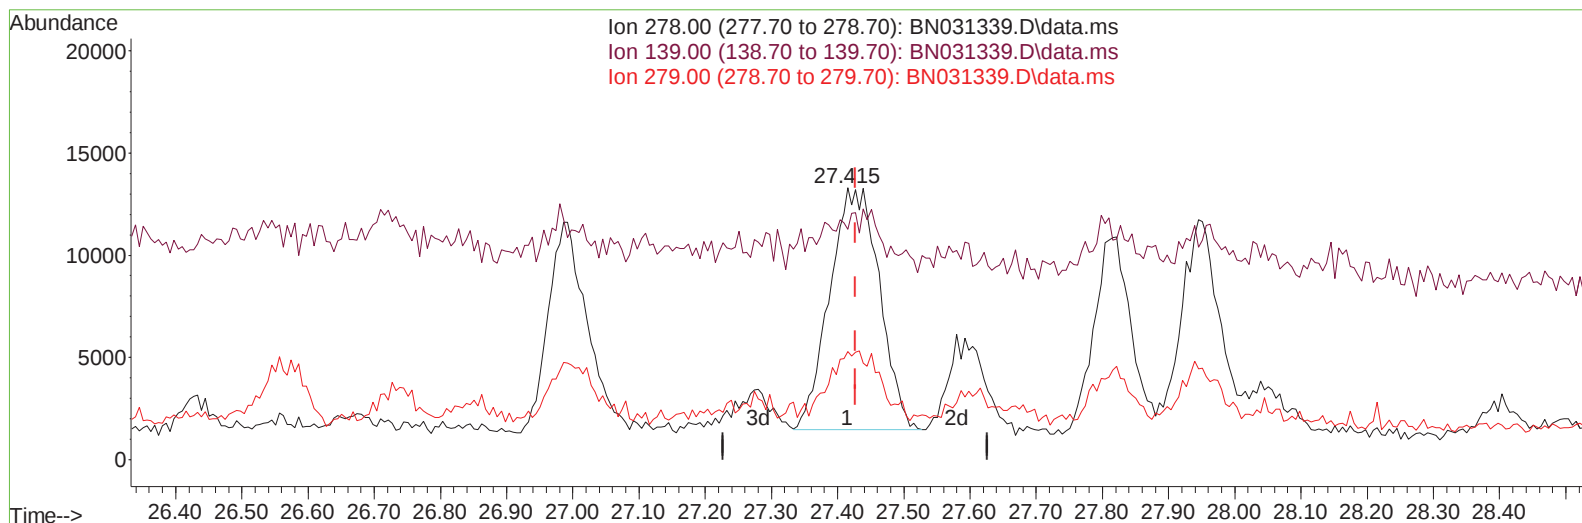

TIC: BN031339.D\data.ms

(95) Dibenzo(a,h)anthracene

27.415min (-0.012) 1.07 ng/ul m

response 61664

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	17.40	84.74#
279.00	23.40	39.72#
0.00	0.00	0.00