




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031340.D
Acq On : 01 May 2024 05:08
Operator : MA/JU
Sample : P2203-20
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CX4

Manual IntegrationsAPPROVED

Quant Time: May 01 05:56:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

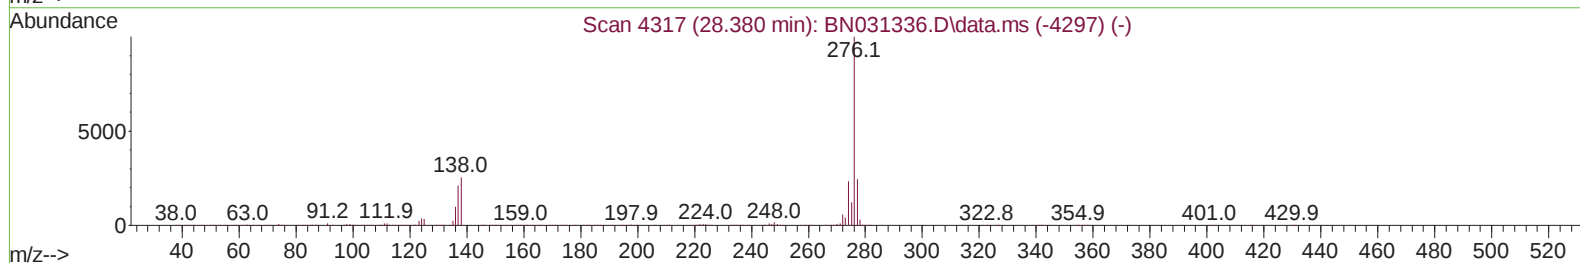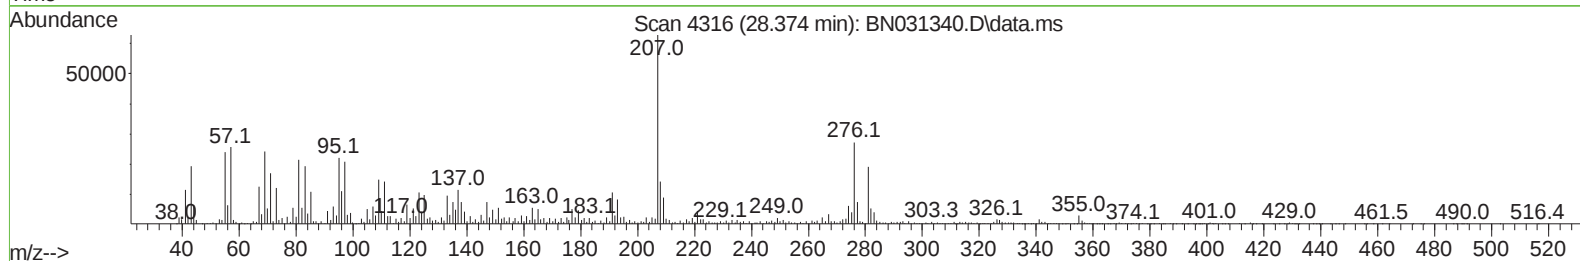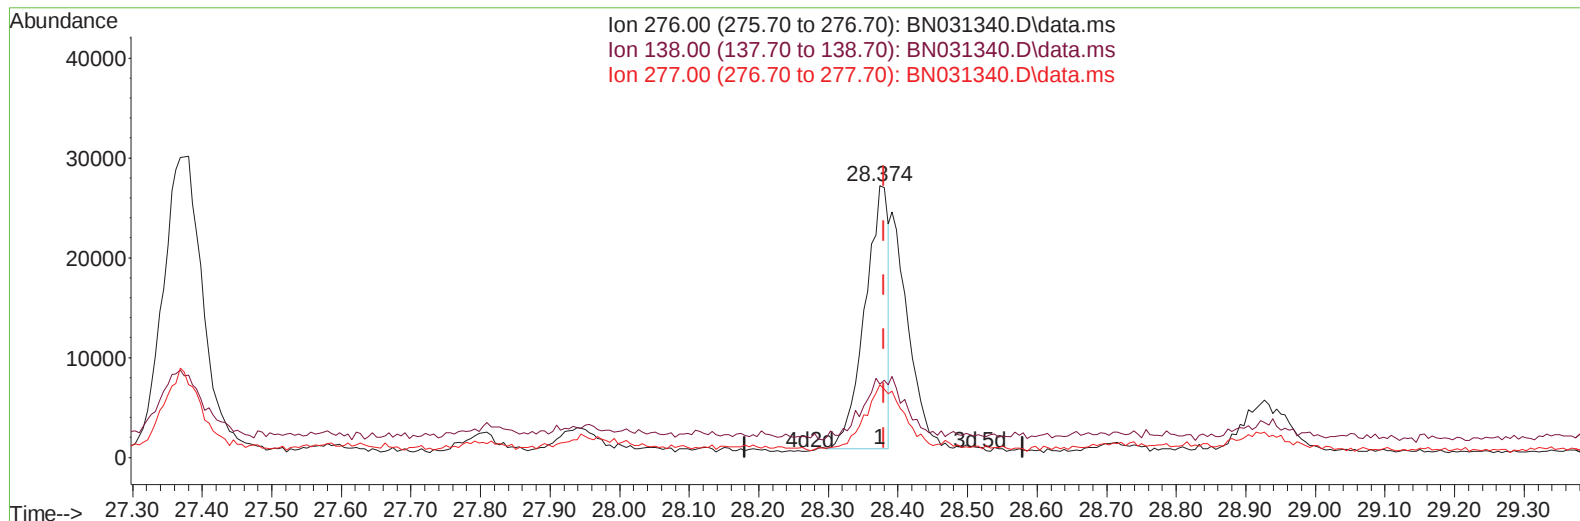

TIC: BN031340.D\data.ms

(96) Benzo(g,h,i)perylene

28.374min (-0.006) 1.13 ng/u1

response 61217

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	23.50	26.99
277.00	22.50	26.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031340.D
 Acq On : 01 May 2024 05:08
 Operator : MA/JU
 Sample : P2203-20
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CX4

Manual IntegrationsAPPROVED

Quant Time: May 01 05:56:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
 Supervised By :mohammad ahmed 05/02/2024

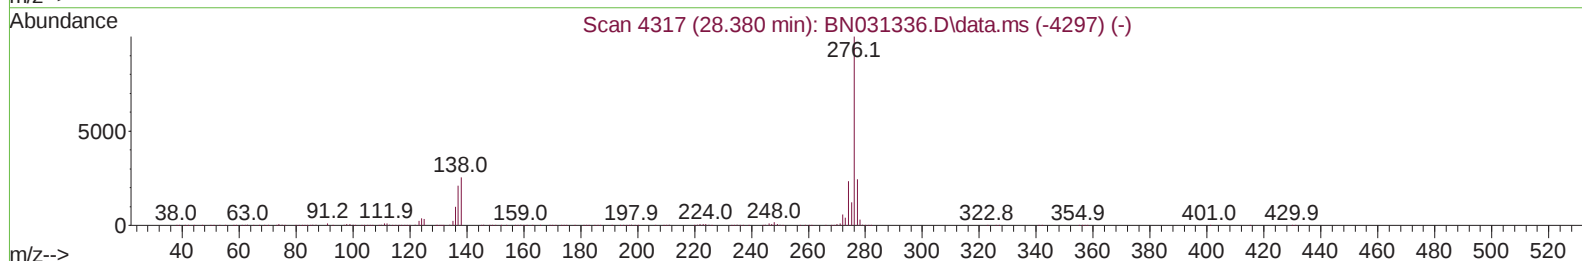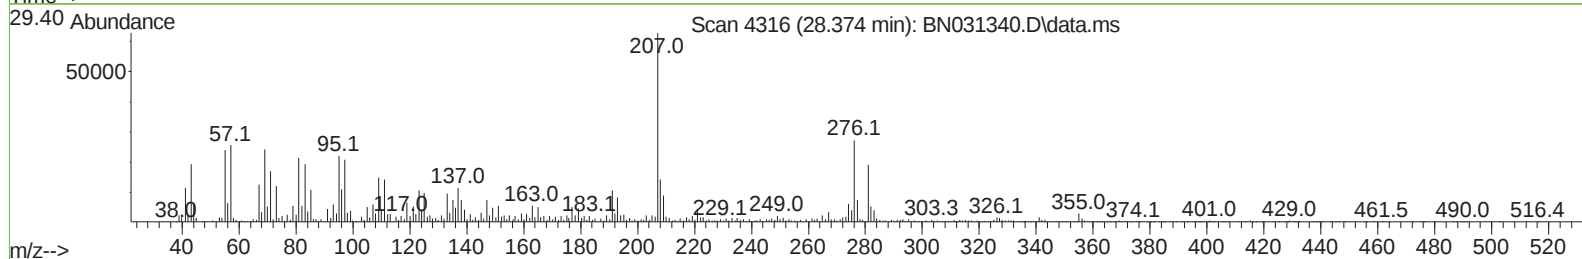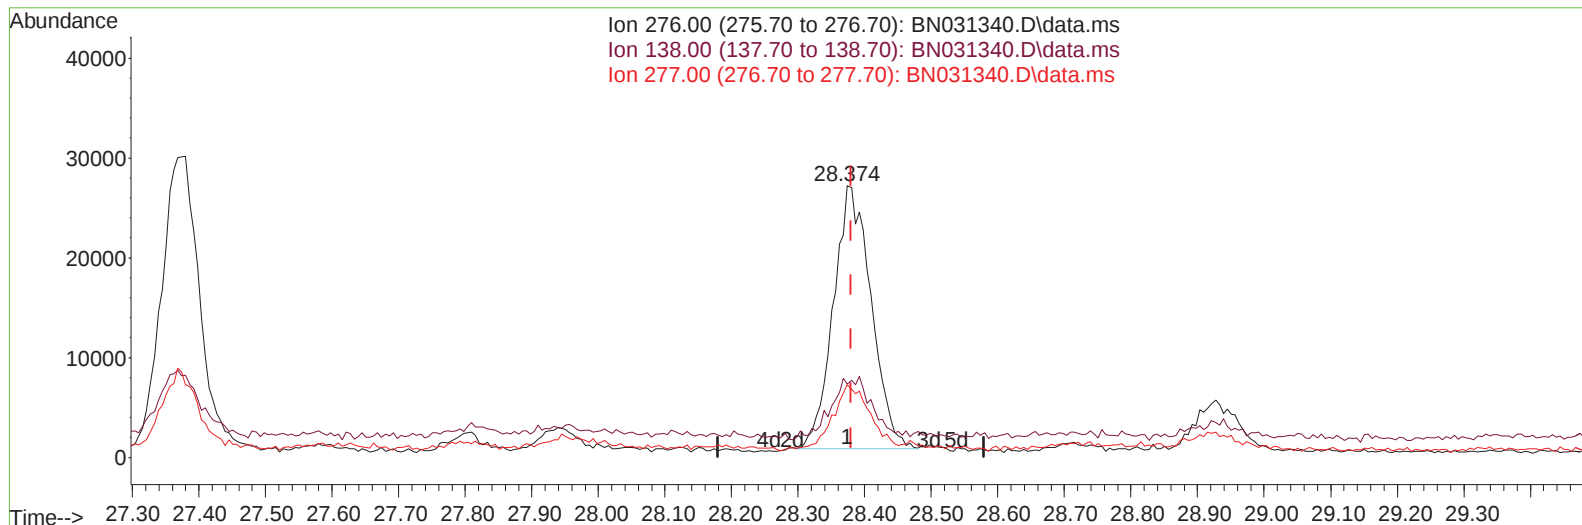

TIC: BN031340.D\data.ms

(96) Benzo(g,h,i)perylene

28.374min (-0.006) 1.91 ng/u1 m

response 103547

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	23.50	26.99
277.00	22.50	26.82
0.00	0.00	0.00