




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031342.D
Acq On : 01 May 2024 06:27
Operator : MA/JU
Sample : P2203-22MSD
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CX4MSD

Manual IntegrationsAPPROVED

Quant Time: May 01 07:54:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

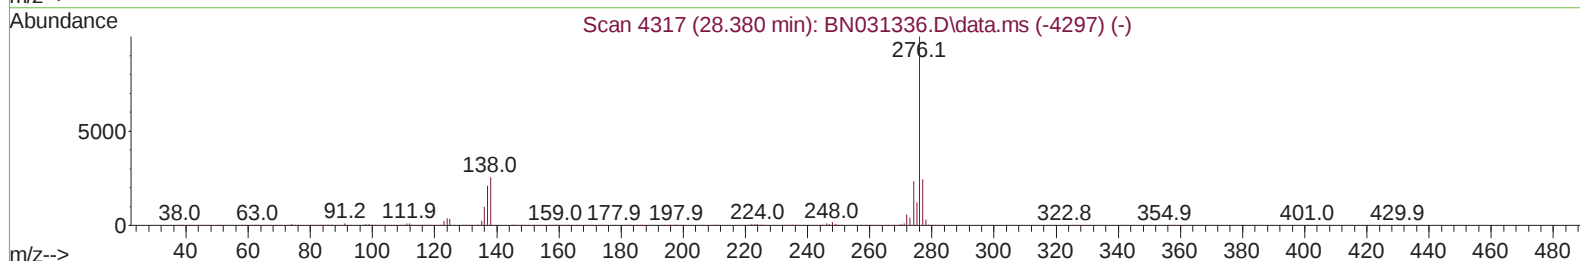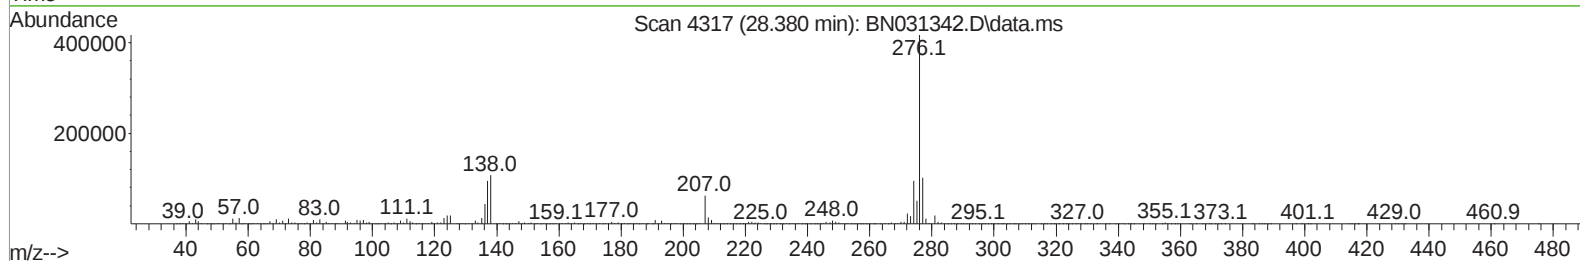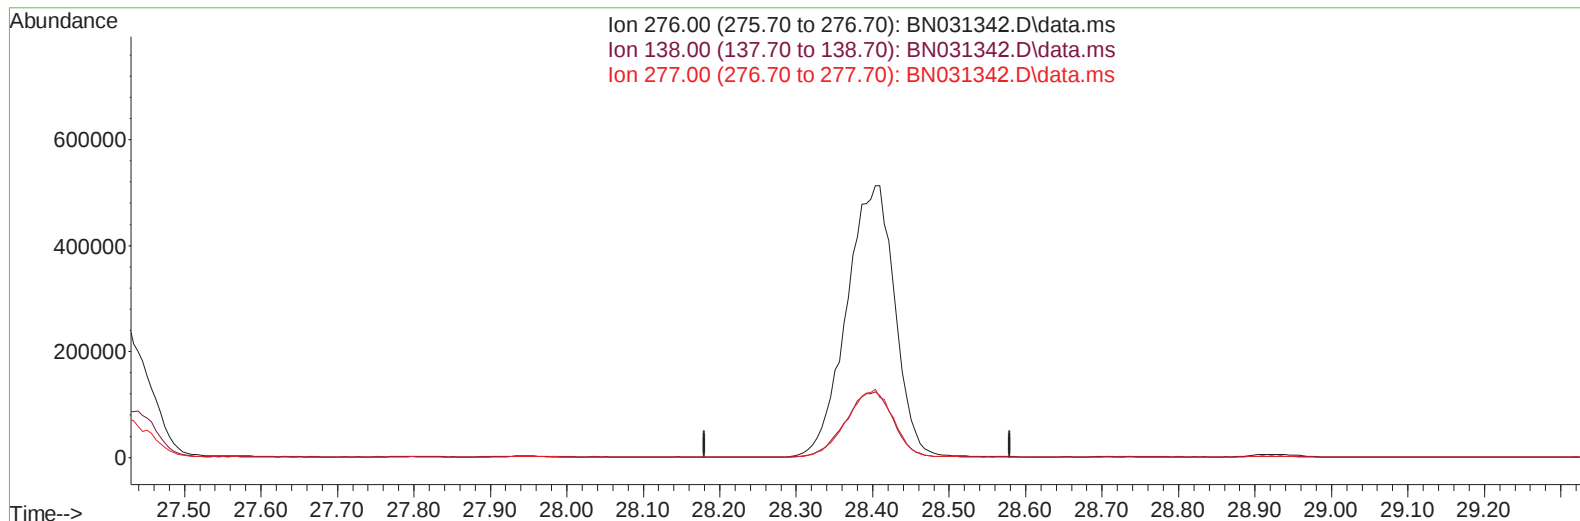

TIC: BN031342.D\data.ms

(96) Benzo(g,h,i)perylene

28.380min (-28.380) 0.00 ng/u1

response 0

Ion	Exp%	Act%
276.00	100.00	0.00
138.00	23.50	0.00#
277.00	22.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031342.D
Acq On : 01 May 2024 06:27
Operator : MA/JU
Sample : P2203-22MSD
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CX4MSD

Manual IntegrationsAPPROVED

Quant Time: May 01 07:54:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/01/2024
Supervised By :mohammad ahmed 05/02/2024

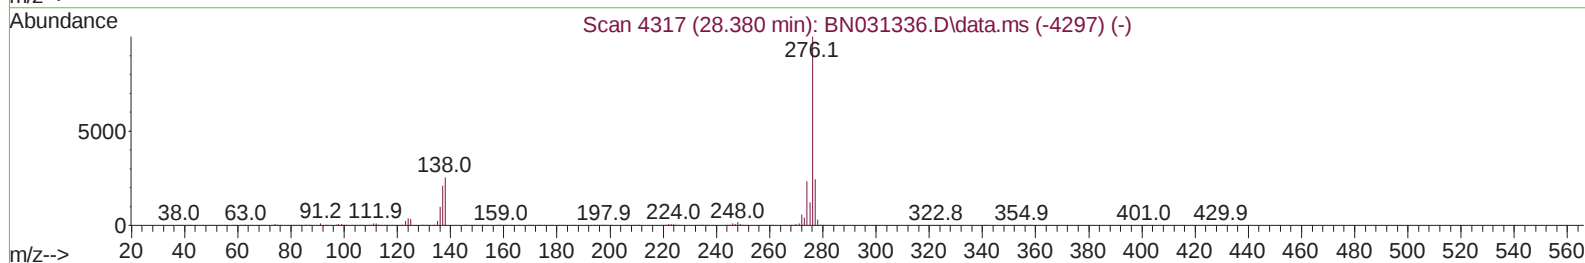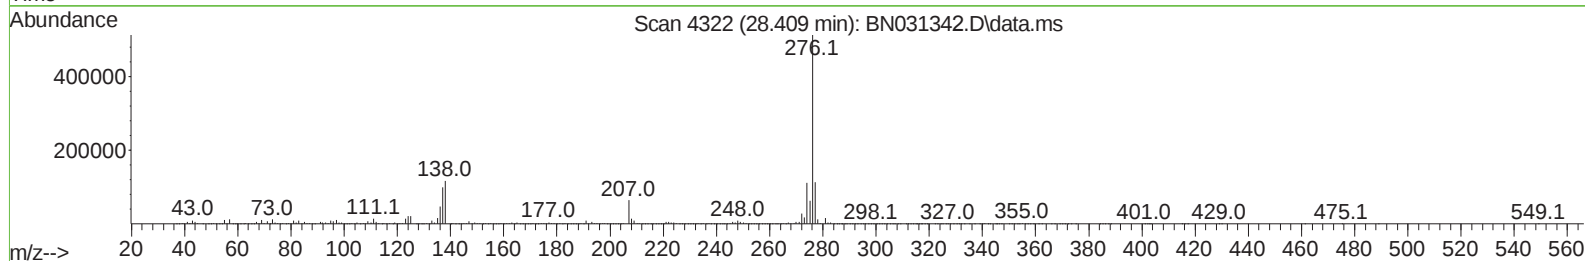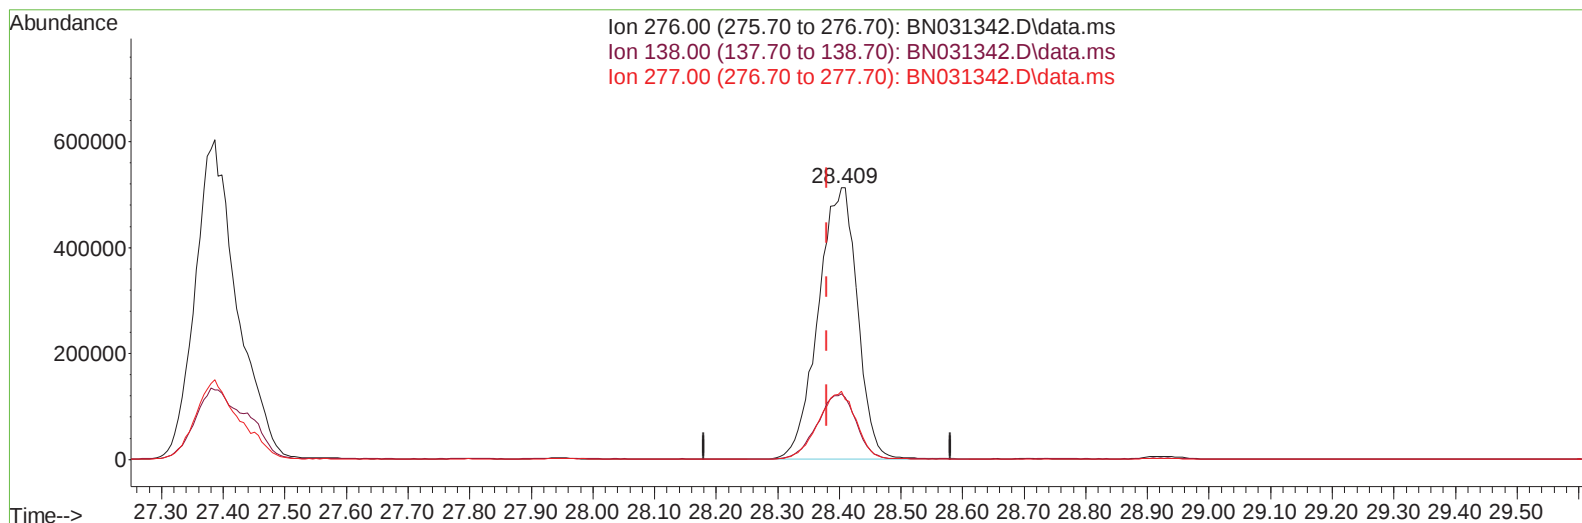

TIC: BN031342.D\data.ms

(96) Benzo(g,h,i)perylene

28.409min (+ 0.030) 50.38 ng/ul m

response 2267955

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	23.50	22.80
277.00	22.50	22.17
0.00	0.00	0.00