

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031325.D
 Acq On : 30 Apr 2024 17:56
 Operator : MA/JU
 Sample : P2161-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R89

Quant Time: Apr 30 23:32:11 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 30 23:30:44 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.617	152	197722	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	871720	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.263	164	596745	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.016	188	1252353	20.000	ng/u1	0.00
79) Chrysene-d12	21.251	240	963245	20.000	ng/u1	0.00
88) Perylene-d12	24.139	264	924743	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	20822	4.903	ng/uL	0.00
4) Pyridine-d5	3.540	84	166094	13.657	ng/u1	0.00
7) Phenol-d5	6.793	99	131654	8.275	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.958	67	412575	44.288	ng/u1	0.00
11) 2-Chlorophenol-d4	7.146	132	411442	32.324	ng/u1	0.00
15) 4-Methylphenol-d8	8.322	113	267082	20.257	ng/u1	0.00
21) Nitrobenzene-d5	8.769	128	290332	46.214	ng/u1	0.00
24) 2-Nitrophenol-d4	9.487	143	291993	43.185	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	504259	40.161	ng/u1	0.00
31) 4-Chloroaniline-d4	10.540	131	736064	40.452	ng/u1	0.00
46) Dimethylphthalate-d6	13.681	166	1898924	48.268	ng/u1	0.00
49) Acenaphthylene-d8	13.951	160	2082013	45.610	ng/u1	0.00
54) 4-Nitrophenol-d4	14.481	143	47459	6.647	ng/u1	0.00
60) Fluorene-d10	15.263	176	1612890	48.009	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.387	200	78966	12.261	ng/u1	0.00
73) Anthracene-d10	17.116	188	2581727	49.951	ng/u1	0.00
81) Pyrene-d10	19.422	212	2933546	50.006	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.945	264	2200544	51.400	ng/u1	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	11.693	107	31497	2.212	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031325.D
Acq On : 30 Apr 2024 17:56
Operator : MA/JU
Sample : P2161-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R89


Quant Time: Apr 30 23:32:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 30 23:30:44 2024
Response via : Initial Calibration

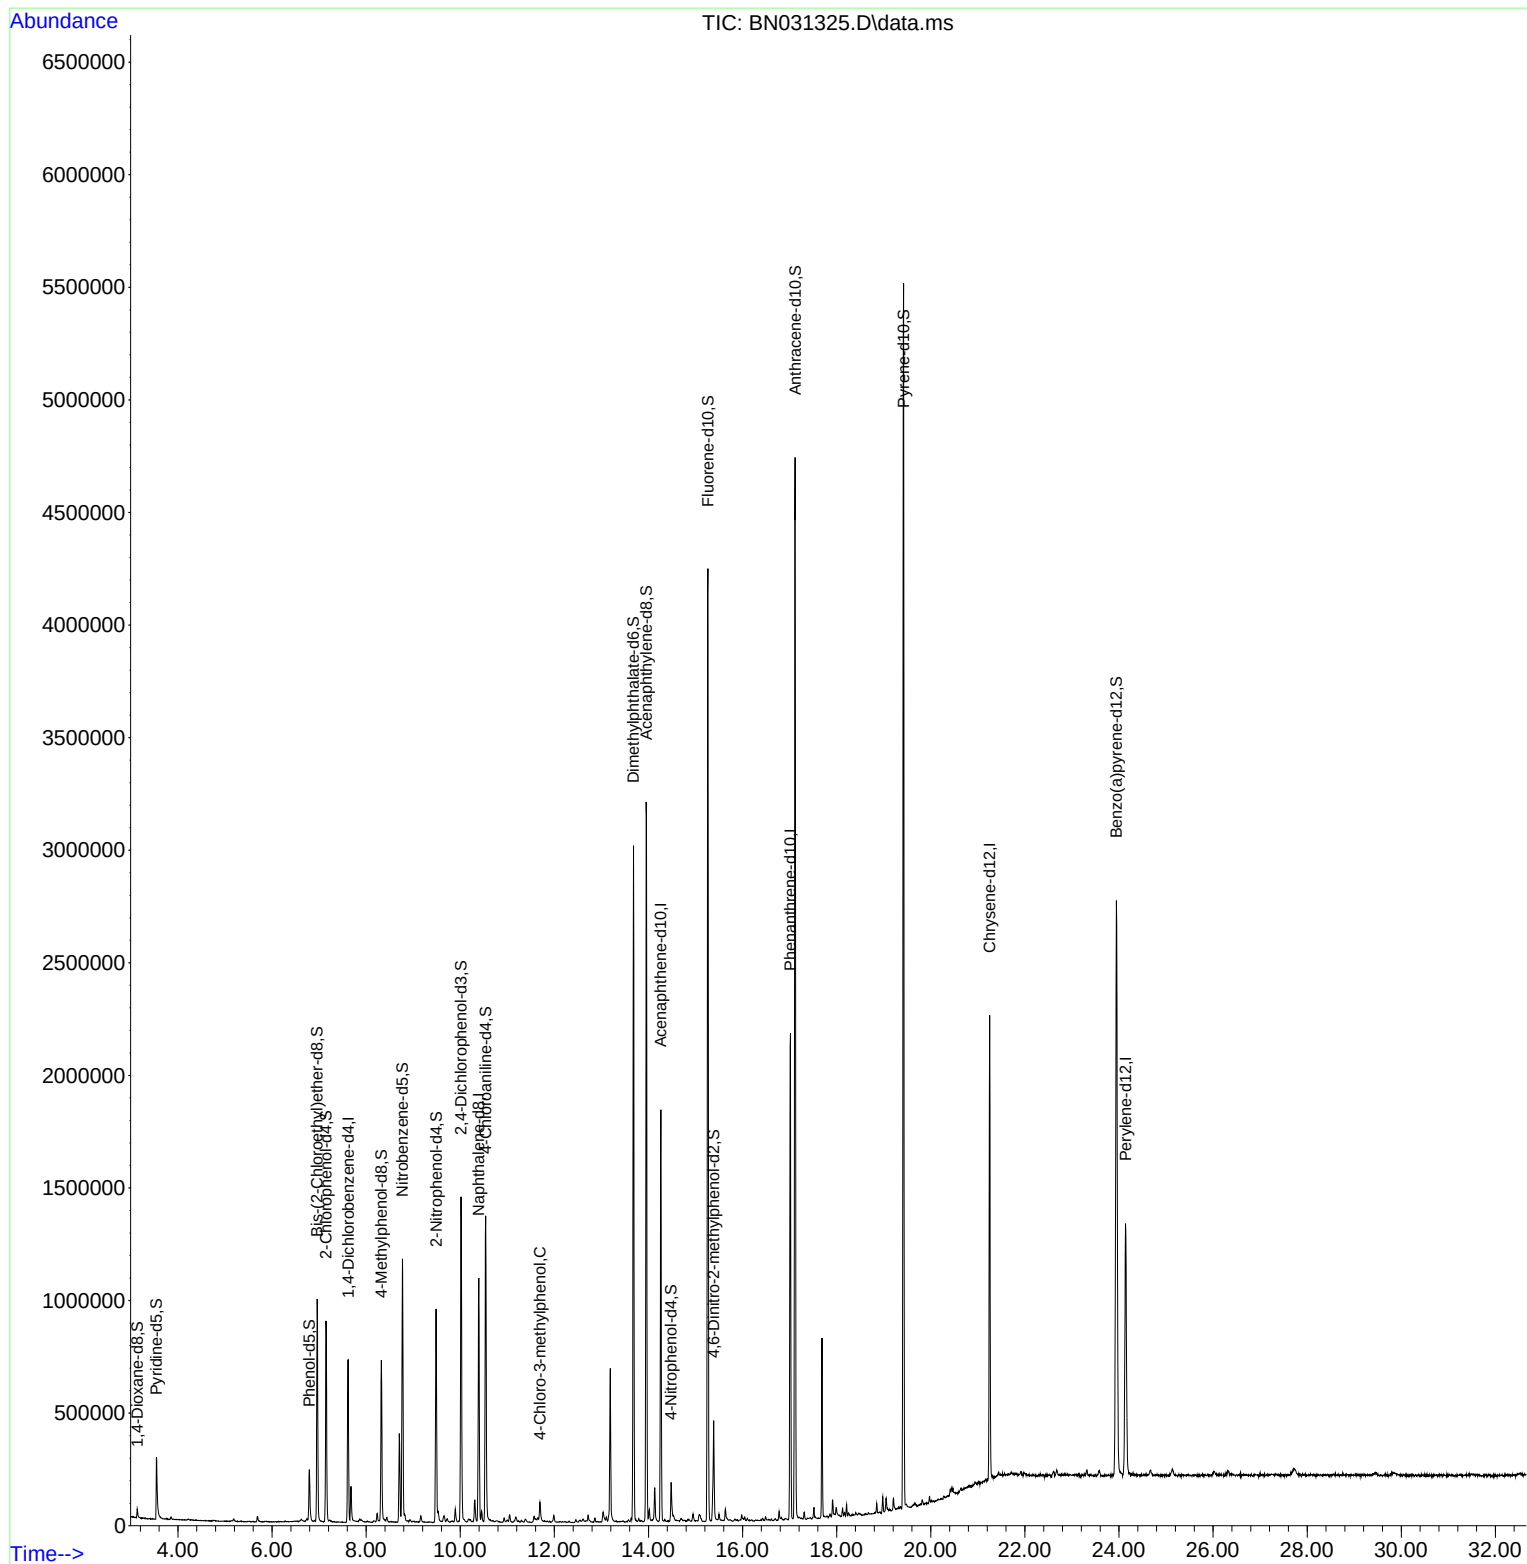

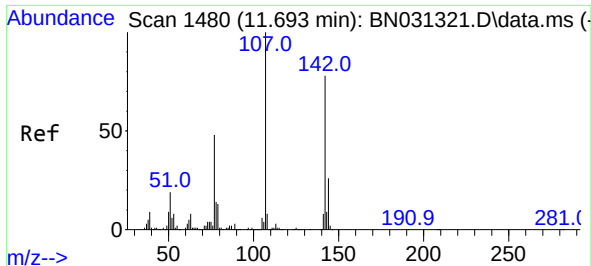

#35
 4-Chloro-3-methylphenol
 Concen: 2.212 ng/ul
 RT: 11.693 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: BN031325.D
 Acq: 30 Apr 2024 17:56

Instrument :
 BNA_N
 ClientSampleId :
 C0R89

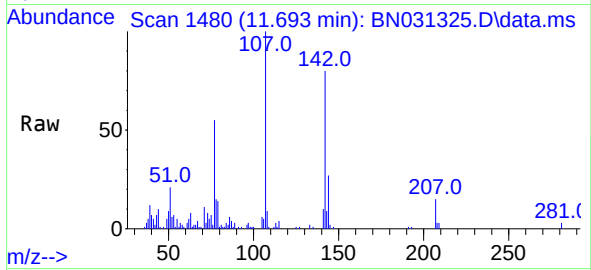

Tgt Ion:	107	Resp:	31497
Ion	Ratio	Lower	Upper
107	100		
144	27.5	20.7	31.1
142	80.4	66.4	99.6

