

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031344.D
 Acq On : 01 May 2024 07:46
 Operator : MA/JU
 Sample : P2203-12
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1CX3

Quant Time: May 01 08:52:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 01 05:16:42 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.610	152	197228	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	890602	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	592970	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.010	188	1209835	20.000	ng/ul	0.00
79) Chrysene-d12	21.245	240	967752	20.000	ng/ul	0.00
88) Perylene-d12	24.133	264	895485	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	24897	5.877	ng/uL	0.00
4) Pyridine-d5	3.534	84	387837	31.970	ng/ul	0.00
7) Phenol-d5	6.787	99	236524	14.903	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.958	67	324058	34.873	ng/ul	0.00
11) 2-Chlorophenol-d4	7.146	132	128001	10.081	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113	386704	29.403	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	243731	37.974	ng/ul	0.00
24) 2-Nitrophenol-d4	9.481	143	56872	8.233	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	112919	8.803	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131	713239	38.367	ng/ul	0.00
46) Dimethylphthalate-d6	13.681	166	1483955	37.960	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	1735809	38.268	ng/ul	0.00
54) 4-Nitrophenol-d4	14.498	143	5696	0.803	ng/ul	0.02
60) Fluorene-d10	15.257	176	1292675	38.723	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	1482	0.238	ng/ul	0.00
73) Anthracene-d10	17.110	188	2001667	40.089	ng/ul	0.00
81) Pyrene-d10	19.416	212	2127154	36.091	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.939	264	1698673	40.974	ng/ul	0.00
Target Compounds						
8) Phenol	6.816	94	31795	1.971	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031344.D
Acq On : 01 May 2024 07:46
Operator : MA/JU
Sample : P2203-12
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1CX3


Quant Time: May 01 08:52:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 01 05:16:42 2024
Response via : Initial Calibration

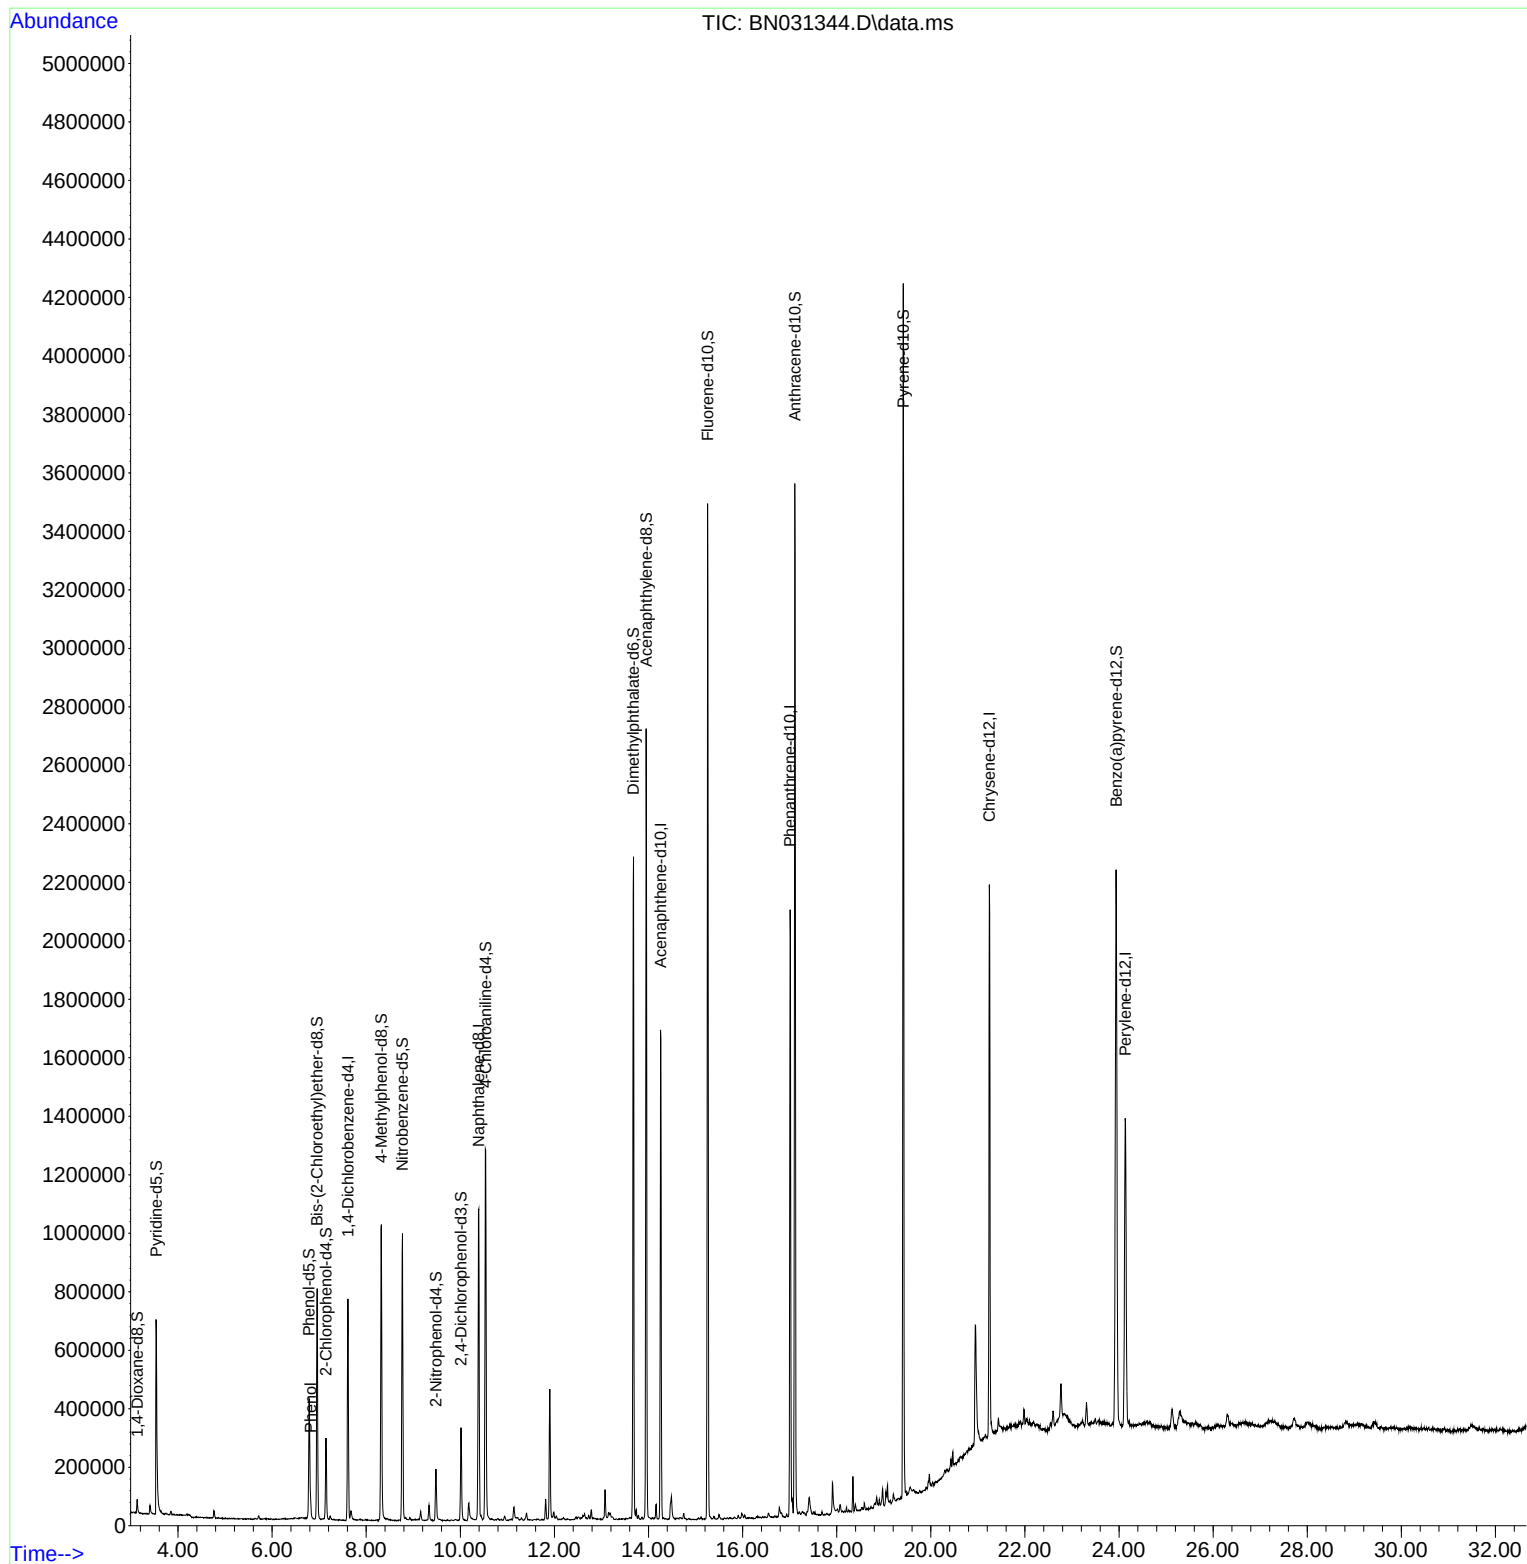

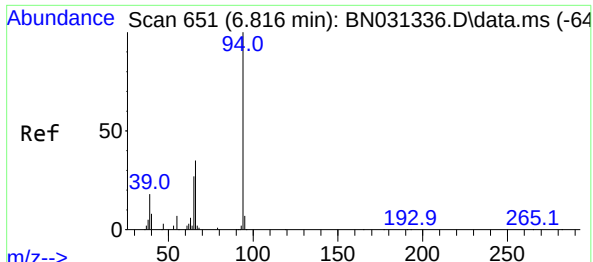

#8
Phenol
Concen: 1.971 ng/ul
RT: 6.816 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN031344.D
Acq: 01 May 2024 07:46

Instrument :
BNA_N
ClientSampleId :
E1CX3

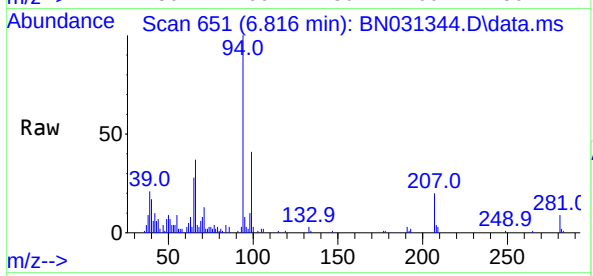

Tgt Ion: 94 Resp: 31795

Ion	Ratio	Lower	Upper
94	100		
65	27.8	21.2	31.8
66	37.2	28.9	43.3

