

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031313.D
 Acq On : 30 Apr 2024 09:06
 Operator : MA/JU
 Sample : PB160530BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK530

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	34	rVB	53671	72100	1.57%	0.133%
2	3.540	91	94	113	rBV	552750	866611	18.85%	1.595%
3	3.852	142	147	152	rVB5	13093	19904	0.43%	0.037%
4	6.746	636	639	641	rBV3	5364	6752	0.15%	0.012%
5	6.793	641	647	666	rVV	869471	1381264	30.05%	2.542%
6	6.958	669	675	687	rVB	701949	1106566	24.07%	2.037%
7	7.146	701	707	715	rBV	861782	1380282	30.03%	2.541%
8	7.616	776	787	798	rBV	846581	1349751	29.36%	2.484%
9	8.322	900	907	919	rBV	1094825	1754177	38.16%	3.229%
10	8.769	975	983	995	rBV	844772	1372909	29.87%	2.527%
11	9.487	1097	1105	1115	rBV	705807	1154516	25.11%	2.125%
12	10.016	1186	1195	1204	rBV	1078503	1823759	39.67%	3.357%
13	10.393	1250	1259	1269	rBV	1248996	2021924	43.98%	3.722%
14	10.540	1275	1284	1304	rBV	903250	1540541	33.51%	2.836%
15	11.987	1525	1530	1538	rBV2	17847	32407	0.70%	0.060%
16	12.604	1630	1635	1641	rBV7	2948	7951	0.17%	0.015%
17	13.157	1724	1729	1734	rBV5	8821	12887	0.28%	0.024%
18	13.228	1736	1741	1744	rVB5	4085	5829	0.13%	0.011%
19	13.681	1811	1818	1832	rBV	2039711	2826223	61.48%	5.202%
20	13.957	1856	1865	1878	rBV	2274786	3432813	74.68%	6.319%
21	14.263	1910	1917	1926	rBV	2051098	2885216	62.76%	5.311%
22	14.481	1948	1954	1977	rBV	795163	1297218	28.22%	2.388%
23	14.675	1983	1987	1993	rVB7	4044	7143	0.16%	0.013%
24	15.063	2048	2053	2054	rBV5	3483	4650	0.10%	0.009%
25	15.263	2080	2087	2101	rBV	2913547	4202870	91.43%	7.736%
26	15.387	2101	2108	2120	rVV	876366	1180427	25.68%	2.173%
27	15.504	2123	2128	2135	rVB2	15592	26896	0.59%	0.050%
28	15.834	2177	2184	2187	rBV9	3271	6092	0.13%	0.011%
29	16.045	2216	2220	2226	rVB4	9641	13123	0.29%	0.024%
30	16.692	2326	2330	2333	rVB5	3957	5447	0.12%	0.010%
31	16.804	2346	2349	2353	rBV5	4611	6586	0.14%	0.012%
32	17.016	2378	2385	2395	rBV	2383384	3357172	73.03%	6.180%
33	17.116	2395	2402	2413	rBV	3095978	4418188	96.11%	8.133%
34	17.916	2531	2538	2548	rBV4	23678	49324	1.07%	0.091%
35	18.980	2714	2719	2723	rBV2	38086	53438	1.16%	0.098%
36	19.051	2727	2731	2735	rVV2	29874	40649	0.88%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031313.D
Acq On : 30 Apr 2024 09:06
Operator : MA/JU
Sample : PB160530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK530

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Title : SVOA CALIBRATION

37	19.210	2754	2758	2762	rBV4	18136	27175	0.59%	0.050%
38	19.416	2787	2793	2802	rBV	3392439	4596968	100.00%	8.462%
39	21.251	3099	3105	3114	rBV	2162486	2909015	63.28%	5.355%
40	23.939	3554	3562	3577	rVB	1725711	4049388	88.09%	7.454%
41	24.139	3588	3596	3609	rVB2	1260233	3021042	65.72%	5.561%




Sum of corrected areas: 54327193

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031313.D
Acq On : 30 Apr 2024 09:06
Operator : MA/JU
Sample : PB160530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK530

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

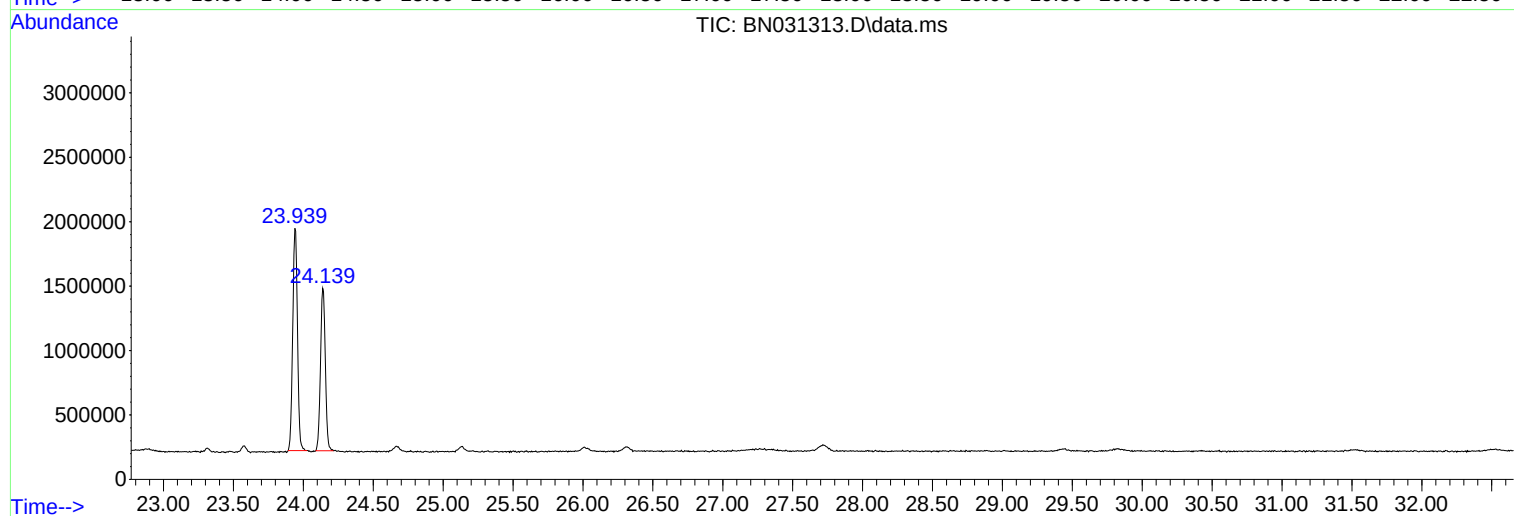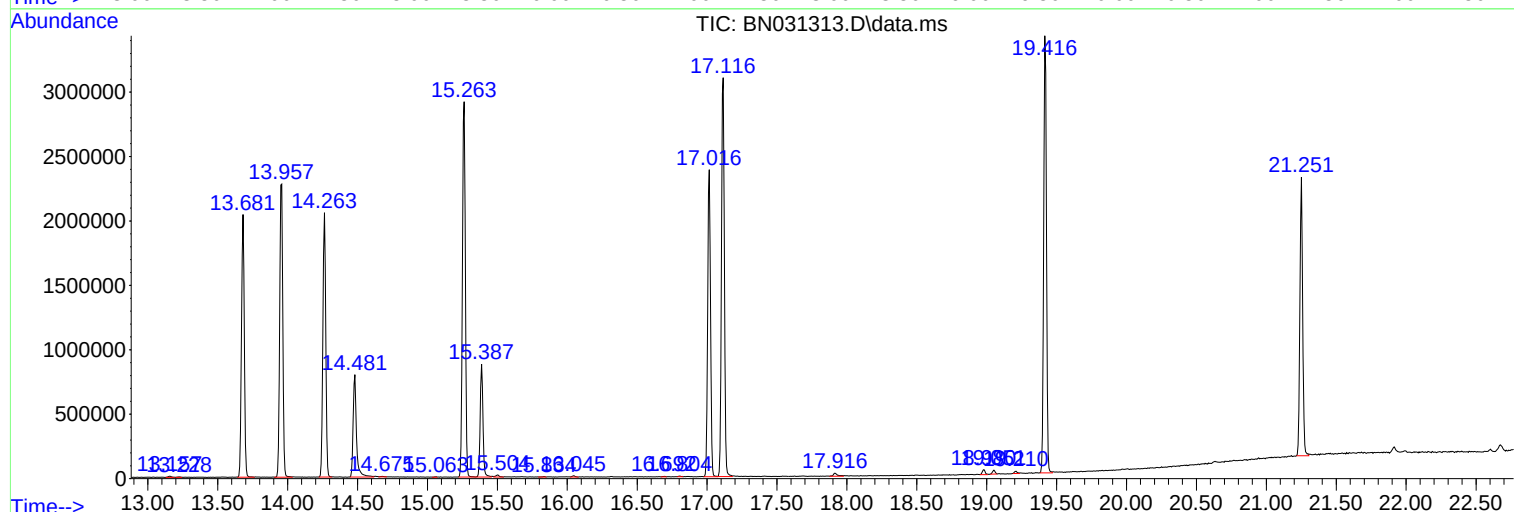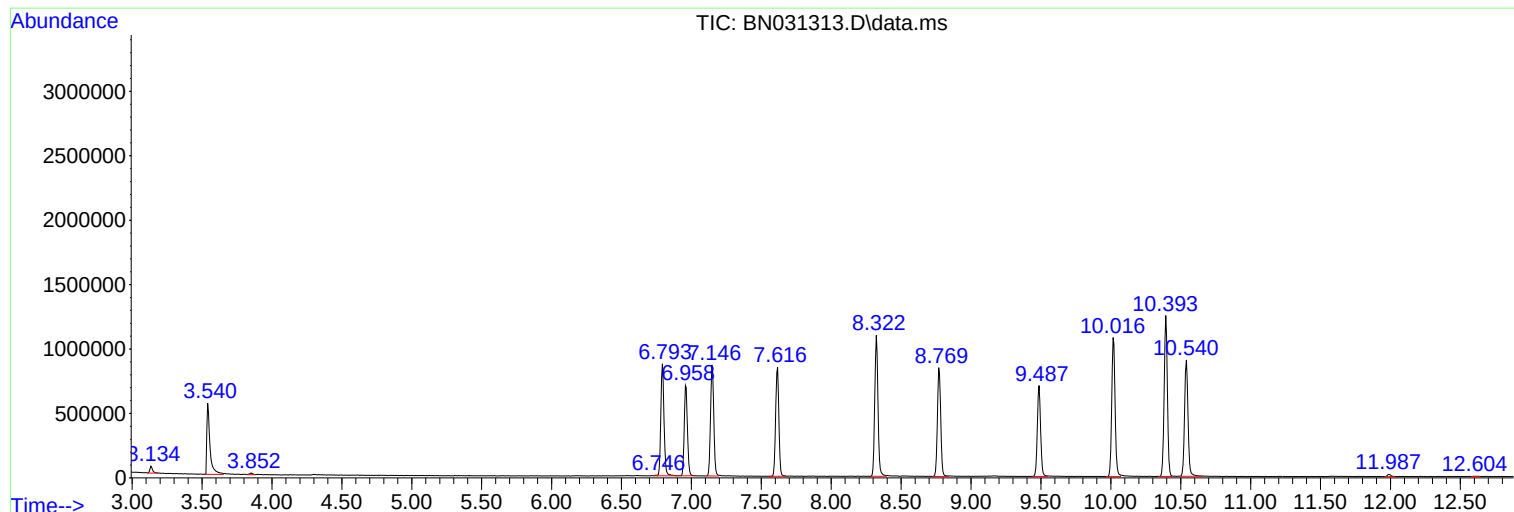

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031313.D
Acq On : 30 Apr 2024 09:06
Operator : MA/JU
Sample : PB160530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK530

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031313.D
Acq On : 30 Apr 2024 09:06
Operator : MA/JU
Sample : PB160530BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK530

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc