

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031323.D
 Acq On : 30 Apr 2024 16:37
 Operator : MA/JU
 Sample : PB160383BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	38	rVB	60476	89785	1.89%	0.157%
2	3.540	91	94	114	rBV	659874	971387	20.50%	1.693%
3	3.852	143	147	152	rVB	16368	20347	0.43%	0.035%
4	4.299	221	223	227	rVB3	4699	5936	0.13%	0.010%
5	6.793	640	647	659	rVB	937311	1455494	30.71%	2.537%
6	6.958	668	675	691	rVB	758374	1178355	24.87%	2.054%
7	7.146	700	707	718	rBV	933134	1469496	31.01%	2.561%
8	7.610	780	786	796	rBV	900743	1435931	30.30%	2.503%
9	8.322	899	907	923	rBV	1197956	1929110	40.71%	3.363%
10	8.769	976	983	996	rBV	928150	1471459	31.05%	2.565%
11	9.487	1097	1105	1115	rBV	776231	1240421	26.18%	2.162%
12	10.016	1187	1195	1212	rBV	1177046	1991773	42.03%	3.472%
13	10.393	1251	1259	1268	rBV	1312399	2159662	45.57%	3.764%
14	10.540	1277	1284	1297	rBV	974361	1685028	35.56%	2.937%
15	11.993	1523	1531	1537	rBV2	19571	36611	0.77%	0.064%
16	13.157	1722	1729	1736	rBV2	14829	23334	0.49%	0.041%
17	13.228	1736	1741	1746	rVB7	3693	6314	0.13%	0.011%
18	13.681	1811	1818	1831	rBV	2369051	3213367	67.81%	5.601%
19	13.951	1857	1864	1876	rBV	2558742	3793310	80.05%	6.612%
20	14.263	1909	1917	1927	rBV	2047031	3012835	63.58%	5.252%
21	14.481	1947	1954	1974	rBV	833783	1405477	29.66%	2.450%
22	15.257	2080	2086	2095	rBV	3156915	4628933	97.68%	8.069%
23	15.387	2102	2108	2120	rBV	896513	1189681	25.10%	2.074%
24	15.498	2122	2127	2132	rVB	16074	26841	0.57%	0.047%
25	16.045	2216	2220	2224	rVB4	10005	13348	0.28%	0.023%
26	16.698	2325	2331	2334	rVB6	5141	8892	0.19%	0.015%
27	16.804	2343	2349	2354	rBV5	5253	8905	0.19%	0.016%
28	17.016	2378	2385	2395	rBV	2346154	3307385	69.79%	5.765%
29	17.110	2395	2401	2413	rVV	3155951	4682990	98.82%	8.163%
30	17.916	2530	2538	2545	rBV8	13301	31324	0.66%	0.055%
31	18.980	2715	2719	2725	rVB4	36895	48975	1.03%	0.085%
32	19.051	2727	2731	2736	rVV	33549	44174	0.93%	0.077%
33	19.204	2755	2757	2765	rVB8	11093	15318	0.32%	0.027%
34	19.416	2787	2793	2807	rBV	3519949	4738929	100.00%	8.260%
35	21.251	3099	3105	3117	rBV	2039551	2843621	60.01%	4.957%
36	23.945	3554	3563	3573	rBV2	1805572	4253663	89.76%	7.414%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031323.D
Acq On : 30 Apr 2024 16:37
Operator : MA/JU
Sample : PB160383BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK383

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Title : SVOA CALIBRATION

37 24.139 3588 3596 3609 rVB 1204346 2931442 61.86% 5.110%




Sum of corrected areas: 57369853

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031323.D
Acq On : 30 Apr 2024 16:37
Operator : MA/JU
Sample : PB160383BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

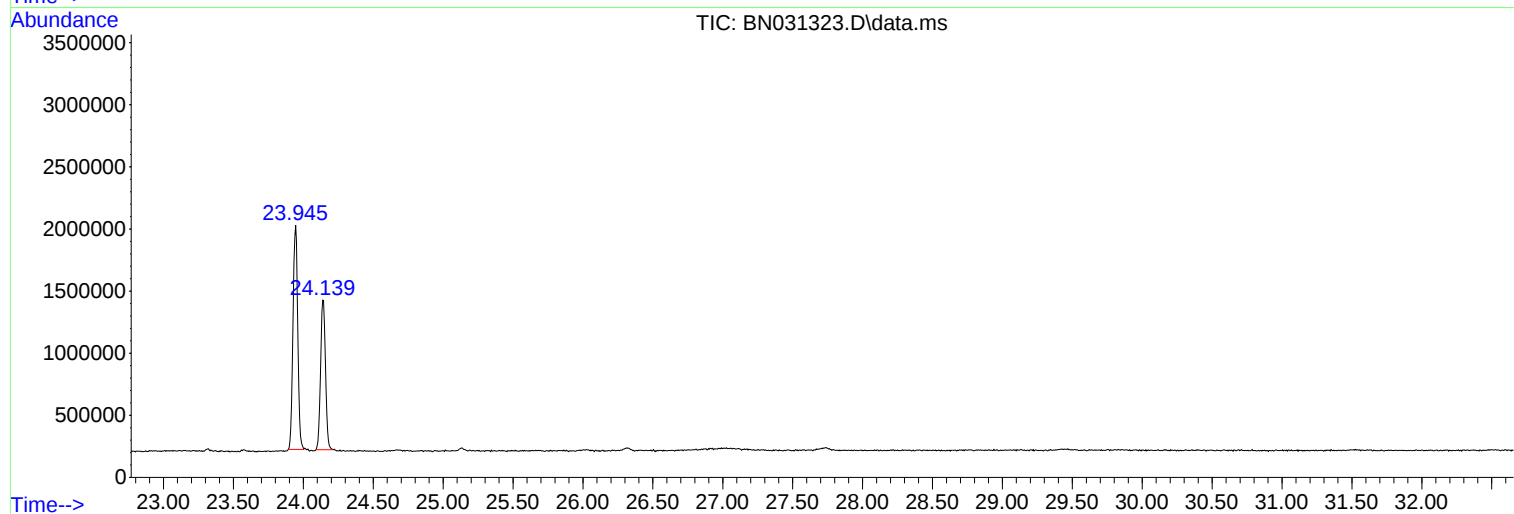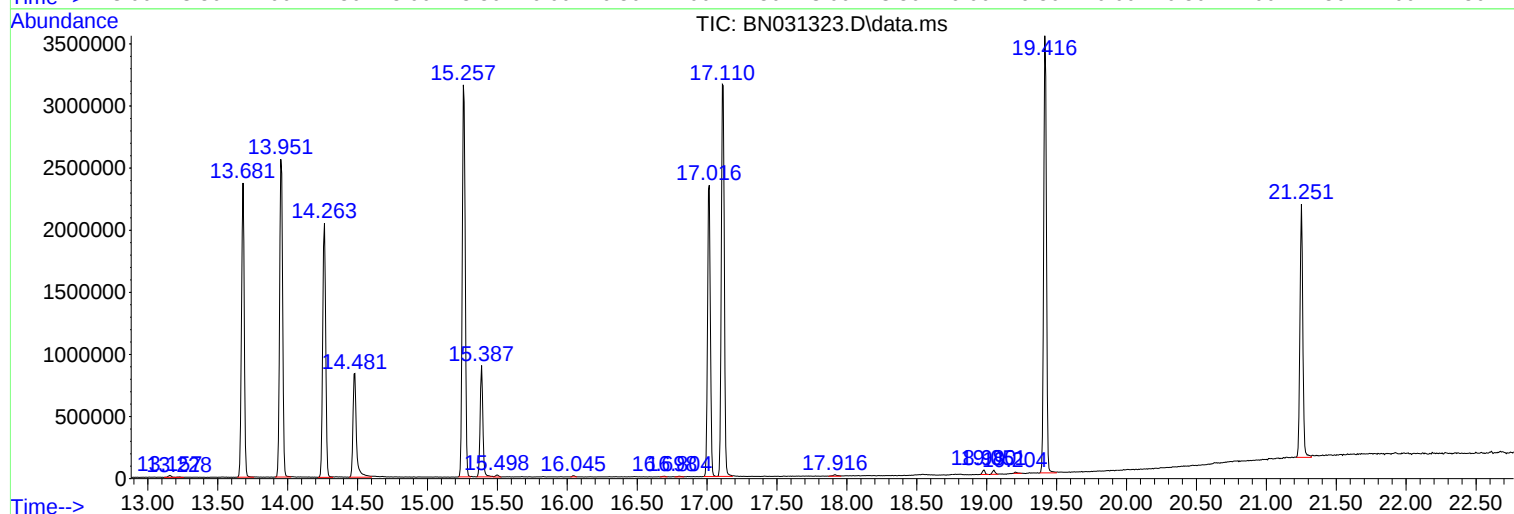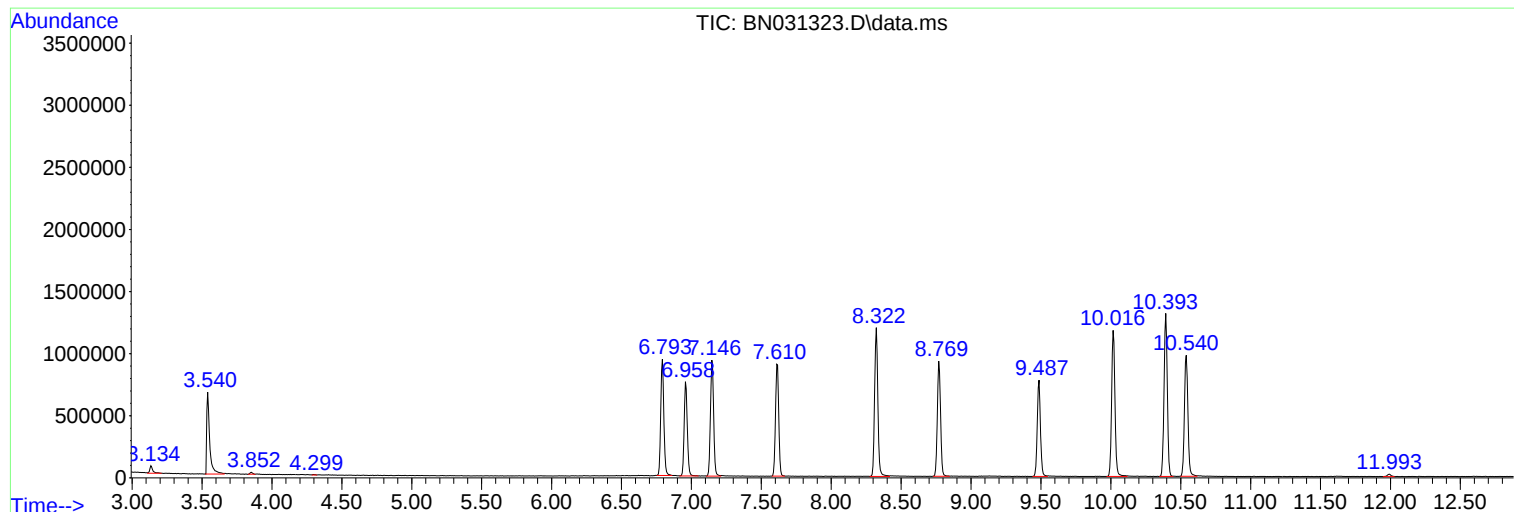

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031323.D
Acq On : 30 Apr 2024 16:37
Operator : MA/JU
Sample : PB160383BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031323.D
Acq On : 30 Apr 2024 16:37
Operator : MA/JU
Sample : PB160383BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK383

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------