

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
 Data File : BN031337.D
 Acq On : 01 May 2024 03:10
 Operator : MA/JU
 Sample : PB160221BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK221

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	34	rVB	77923	102135	1.82%	0.144%
2	3.540	91	94	109	rBV	743933	1123701	20.06%	1.581%
3	3.852	143	147	153	rVB2	16728	21893	0.39%	0.031%
4	6.740	636	638	640	rBV3	6468	8282	0.15%	0.012%
5	6.787	640	646	660	rVB	1190132	1886222	33.67%	2.653%
6	6.958	669	675	689	rVB	994567	1517007	27.08%	2.134%
7	7.146	698	707	720	rBV	1202373	1909379	34.08%	2.686%
8	7.610	778	786	797	rBV	1177254	1829651	32.66%	2.573%
9	8.322	898	907	919	rBV	1479447	2410116	43.02%	3.390%
10	8.769	976	983	993	rBV	1183876	1877305	33.51%	2.640%
11	8.922	1008	1009	1015	rVB6	4817	6997	0.12%	0.010%
12	9.169	1045	1051	1059	rVB8	6485	14851	0.27%	0.021%
13	9.481	1097	1104	1115	rBV	961474	1598303	28.53%	2.248%
14	10.016	1188	1195	1209	rBV	1504507	2491439	44.47%	3.504%
15	10.393	1251	1259	1269	rBV	1659257	2764096	49.34%	3.888%
16	10.534	1276	1283	1303	rBV	1374247	2388956	42.64%	3.360%
17	11.651	1468	1473	1479	rVB8	4178	7965	0.14%	0.011%
18	11.987	1524	1530	1538	rBV3	24757	42772	0.76%	0.060%
19	12.604	1629	1635	1640	rVB8	4737	8405	0.15%	0.012%
20	13.151	1723	1728	1736	rVB2	14886	25783	0.46%	0.036%
21	13.228	1736	1741	1743	rBV3	4894	6663	0.12%	0.009%
22	13.681	1811	1818	1829	rBV	2638049	3667255	65.46%	5.158%
23	13.951	1857	1864	1878	rBV2	3087750	4548600	81.19%	6.398%
24	14.257	1908	1916	1929	rBV	2496818	3806949	67.95%	5.355%
25	14.475	1947	1953	1977	rBV	1021655	1637983	29.24%	2.304%
26	14.675	1983	1987	1991	rVB6	5753	7997	0.14%	0.011%
27	15.057	2048	2052	2057	rVB7	4015	6774	0.12%	0.010%
28	15.257	2078	2086	2093	rBV	3690394	5383816	96.10%	7.572%
29	15.386	2101	2108	2119	rBV	1099409	1539629	27.48%	2.166%
30	15.498	2122	2127	2133	rVB2	19750	30527	0.54%	0.043%
31	16.045	2216	2220	2226	rVB6	12260	18627	0.33%	0.026%
32	16.692	2327	2330	2334	rVB5	6942	8521	0.15%	0.012%
33	16.798	2344	2348	2351	rBV3	8465	10646	0.19%	0.015%
34	17.010	2378	2384	2395	rBV	2934213	4180086	74.61%	5.879%
35	17.110	2395	2401	2413	rVV2	3839973	5463648	97.52%	7.685%
36	17.310	2431	2435	2438	rVB6	4069	5633	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031337.D
Acq On : 01 May 2024 03:10
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK221

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Title : SVOA CALIBRATION

37	17.675	2495	2497	2502	rVB4	4700	7887	0.14%	0.011%
38	17.910	2533	2537	2544	rBV7	18531	26248	0.47%	0.037%
39	18.975	2713	2718	2724	rBV2	46178	66363	1.18%	0.093%
40	19.045	2726	2730	2735	rBV	40331	54376	0.97%	0.076%
41	19.204	2754	2757	2762	rBV7	16291	20470	0.37%	0.029%
42	19.304	2771	2774	2777	rBV4	7028	10236	0.18%	0.014%
43	19.416	2787	2793	2802	rBV	4150620	5602317	100.00%	7.880%
44	21.245	3099	3104	3113	rBV	2572182	3578587	63.88%	5.033%
45	23.939	3553	3562	3576	rVB2	2278326	5287410	94.38%	7.437%
46	24.139	3587	3596	3606	rBV	1746712	4084457	72.91%	5.745%




Sum of corrected areas: 71096963

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031337.D
Acq On : 01 May 2024 03:10
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

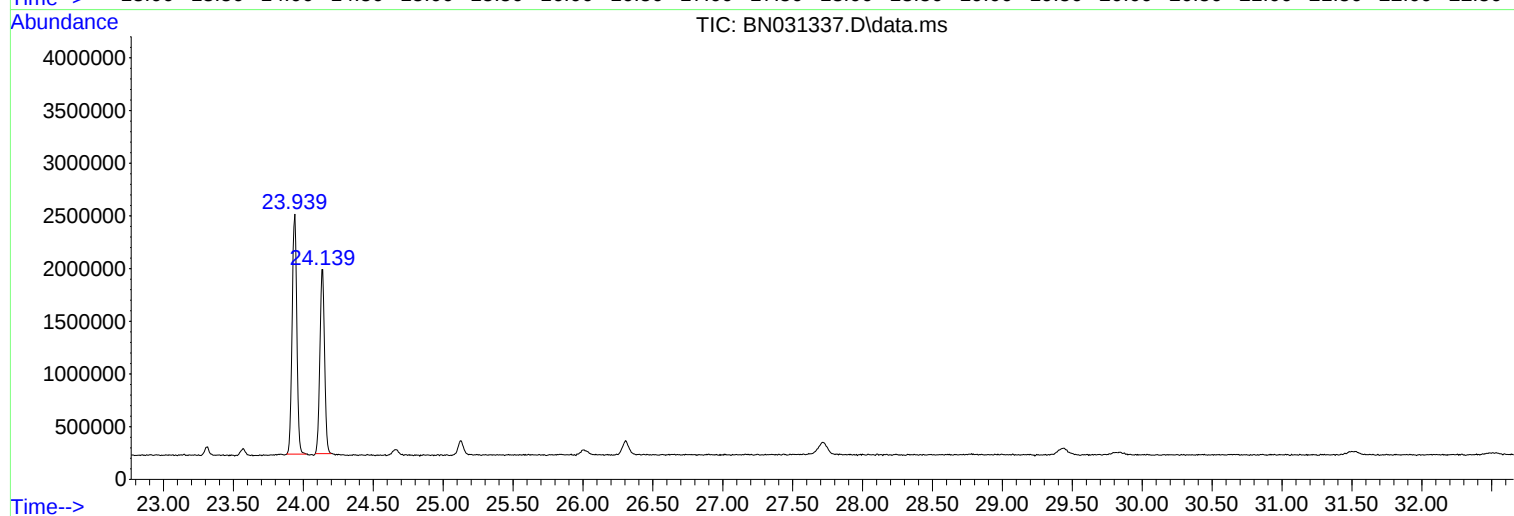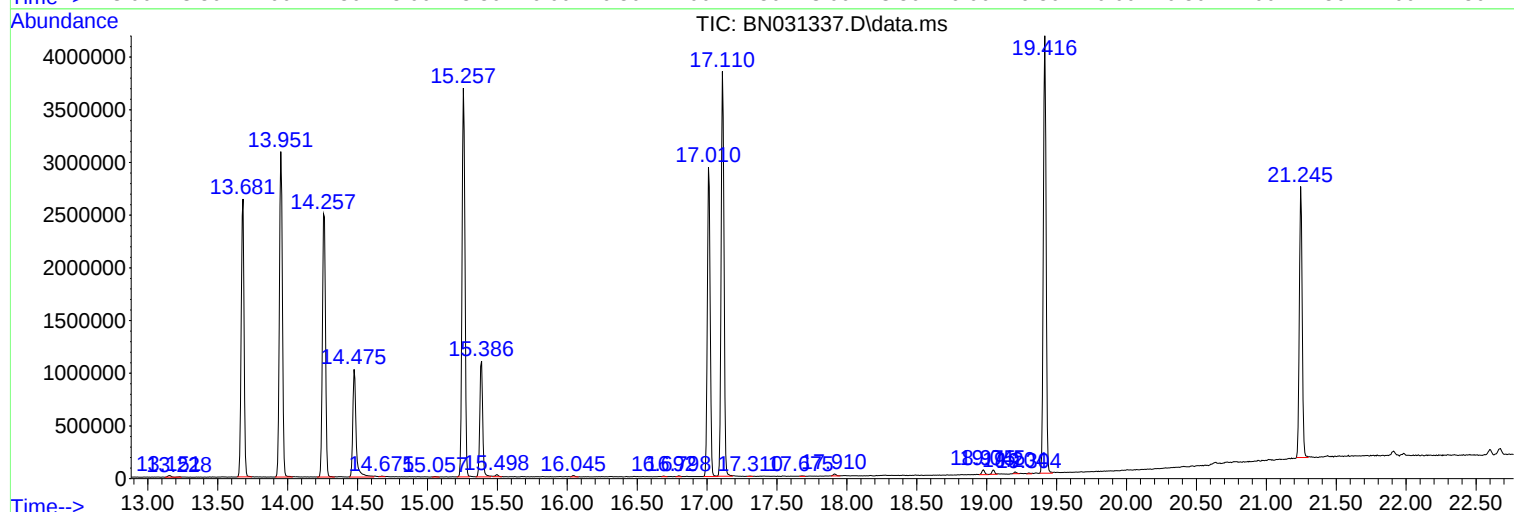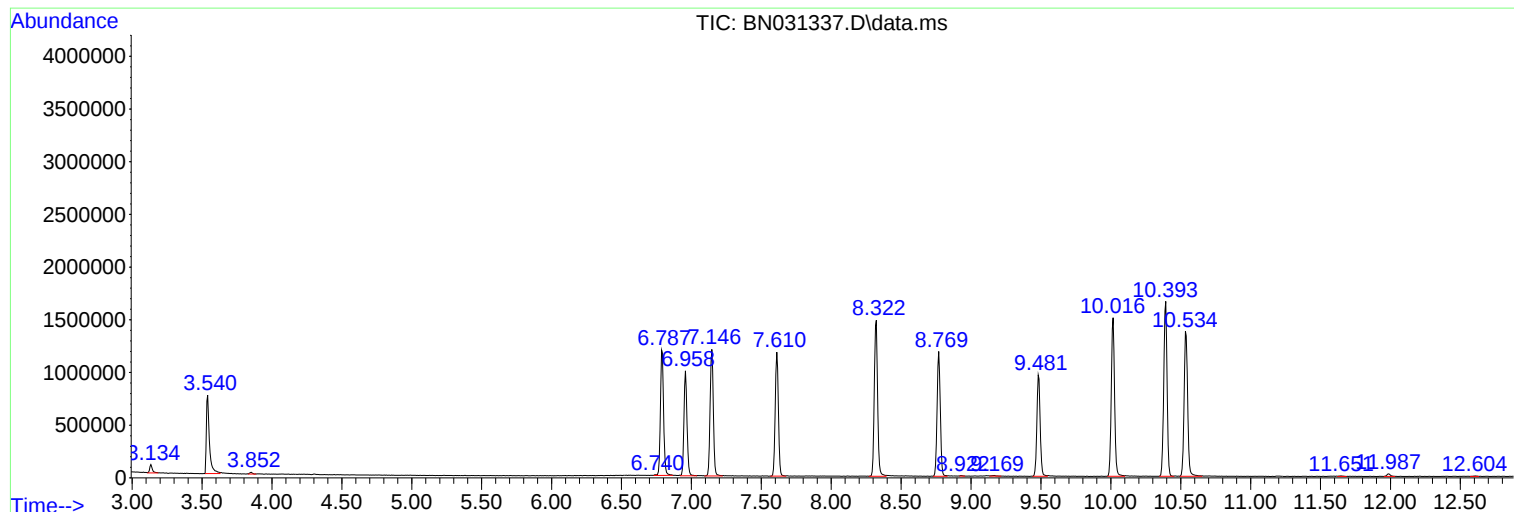

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031337.D
Acq On : 01 May 2024 03:10
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043024\
Data File : BN031337.D
Acq On : 01 May 2024 03:10
Operator : MA/JU
Sample : PB160221BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK221

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------