
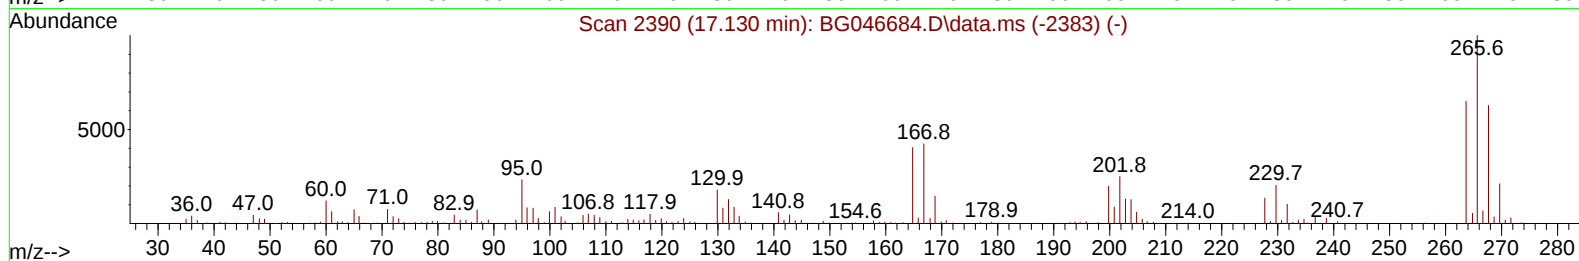
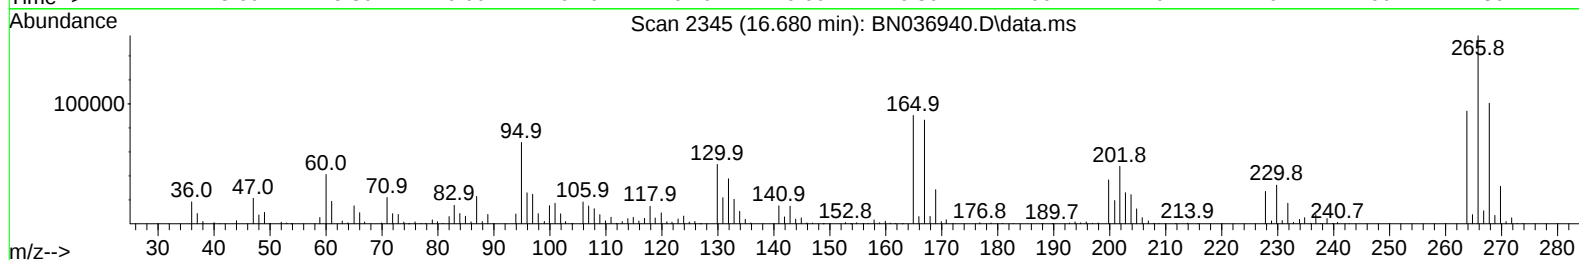


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043025\
Data File : BN036940.D
Acq On : 30 Apr 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 17:05:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

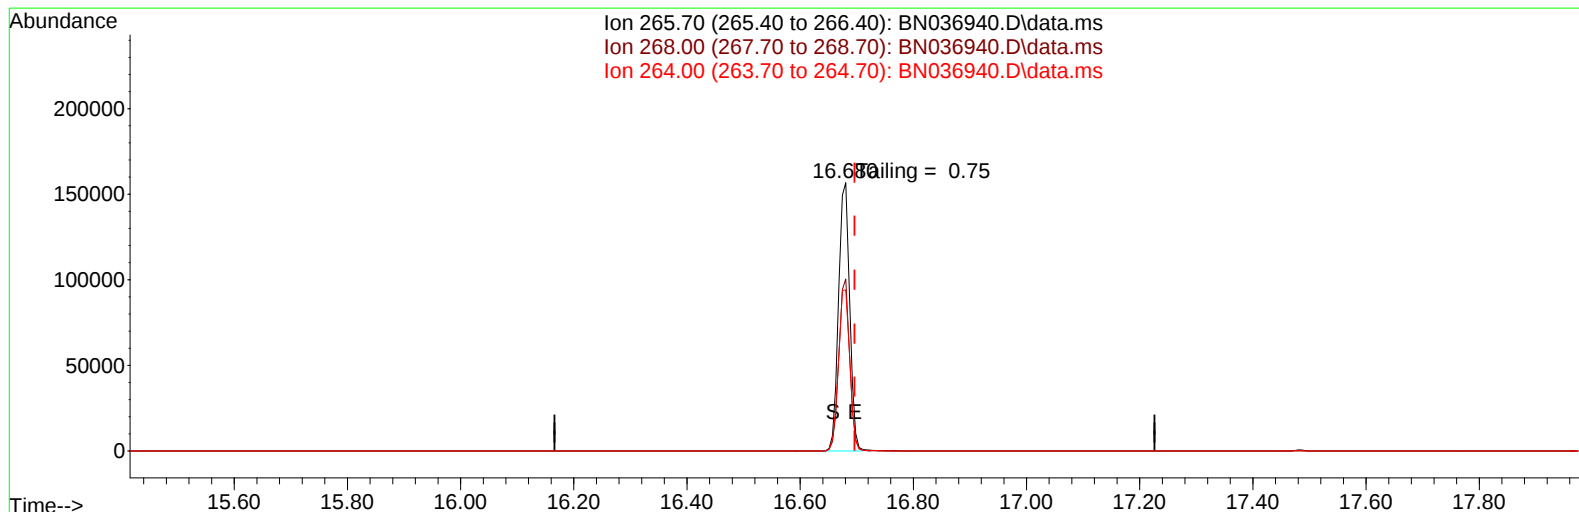

TIC: BN036940.D\data.ms

(70) Pentachlorophenol (C)




16.680min (-0.016) 16606.24 ng

response 213988

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.09
264.00	61.60	59.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN043025\
Data File : BN036940.D
Acq On : 30 Apr 2025 10:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 17:05:48 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 11 23:51:57 2025
Response via : Initial Calibration

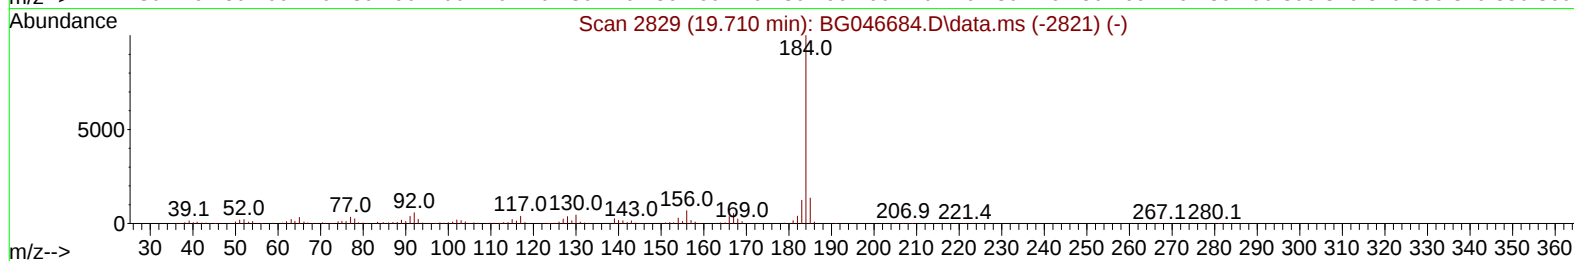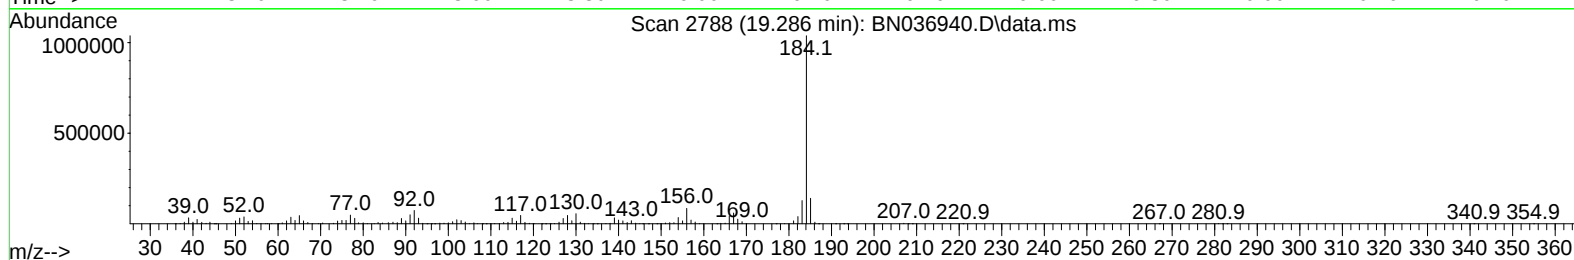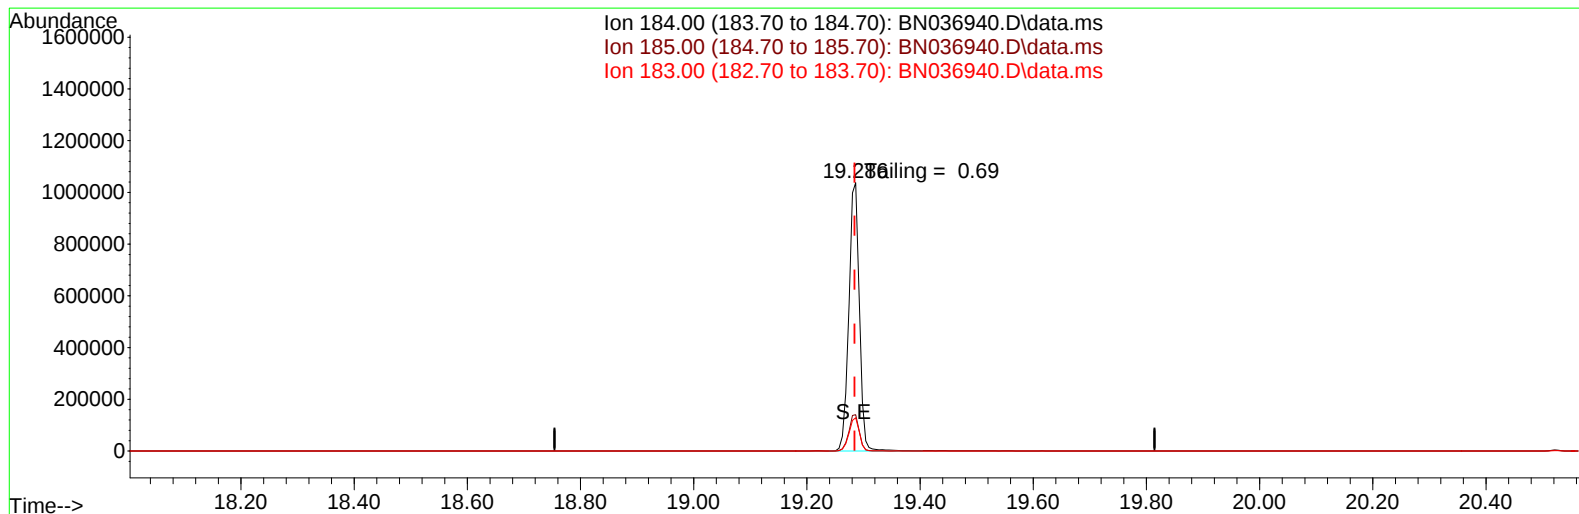

TIC: BN036940.D\data.ms

(77) Benzidine

19.286min (+ 0.002) 0.00 ng

response 1344463

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.57
183.00	13.20	12.39
0.00	0.00	0.00