

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050119\
 Data File : BN005404.D
 Acq On : 01 May 2019 11:19
 Operator : JU/SJ
 Sample : PB119345BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	35	39	45	rVB	115350	141069	1.51%	0.133%
2	3.917	154	158	163	rVB3	19725	28537	0.31%	0.027%
3	6.775	637	644	658	rBV	1822465	2833542	30.33%	2.670%
4	6.940	665	672	687	rVB	1423051	2181635	23.35%	2.056%
5	7.128	698	704	717	rBV	1816655	2921320	31.27%	2.753%
6	7.593	775	783	794	rBV	1620586	2566339	27.47%	2.418%
7	8.293	894	902	916	rBV	2302596	3646603	39.04%	3.436%
8	8.734	968	977	989	rBV	1779618	2888804	30.92%	2.722%
9	9.446	1090	1098	1108	rBV	1463854	2466406	26.40%	2.324%
10	9.981	1180	1189	1208	rBV	2237668	3833952	41.04%	3.613%
11	10.352	1243	1252	1260	rBV	2264558	3688532	39.48%	3.476%
12	10.493	1268	1276	1289	rBV	2196496	3820388	40.90%	3.600%
13	11.957	1515	1525	1534	rBV4	24523	67752	0.73%	0.064%
14	13.193	1728	1735	1740	rVB5	7634	15582	0.17%	0.015%
15	13.645	1805	1812	1822	rVB	4244124	5900854	63.17%	5.561%
16	13.916	1850	1858	1873	rBV	4709798	6947515	74.37%	6.547%
17	14.069	1877	1884	1893	rBV2	41321	113086	1.21%	0.107%
18	14.228	1903	1911	1921	rVB2	3294887	4950095	52.99%	4.665%
19	14.440	1940	1947	1970	rBV	1371242	2708458	28.99%	2.552%
20	15.228	2074	2081	2089	rBV	5909727	8436616	90.31%	7.950%
21	15.357	2097	2103	2117	rBV	1466660	2308308	24.71%	2.175%
22	15.463	2117	2121	2127	rVB2	80762	118161	1.26%	0.111%
23	15.792	2170	2177	2184	rBV4	7551	15936	0.17%	0.015%
24	16.010	2210	2214	2223	rBV4	22994	35829	0.38%	0.034%
25	16.181	2239	2243	2248	rBV4	6385	10636	0.11%	0.010%
26	16.657	2321	2324	2330	rVB3	8842	10202	0.11%	0.010%
27	16.763	2338	2342	2350	rVB3	17163	27701	0.30%	0.026%
28	16.981	2372	2379	2389	rBV2	3903735	5689086	60.90%	5.361%
29	17.081	2389	2396	2413	rVB2	6078514	9002274	96.37%	8.483%
30	17.910	2532	2537	2541	rBV6	12369	23282	0.25%	0.022%
31	19.028	2722	2727	2731	rBV	59008	79070	0.85%	0.075%
32	19.198	2754	2756	2763	rBV8	6793	12786	0.14%	0.012%
33	19.280	2765	2770	2776	rVB	52217	73029	0.78%	0.069%
34	19.392	2779	2789	2806	rBV	6662774	9341605	100.00%	8.803%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050119\
Data File : BN005404.D
Acq On : 01 May 2019 11:19
Operator : JU/SJ
Sample : PB119345BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Title : SVOA CALIBRATION

35	20.016	2892	2895	2901	rBV7	8633	17528	0.19%	0.017%
36	21.210	3092	3098	3109	rBV	3681052	4864715	52.08%	4.584%
37	21.392	3126	3129	3138	rBV3	53549	110346	1.18%	0.104%
38	21.827	3199	3203	3208	rBV3	74728	100731	1.08%	0.095%
39	22.280	3277	3280	3285	rVB	159417	184640	1.98%	0.174%
40	22.780	3361	3365	3374	rVB	211560	297419	3.18%	0.280%
41	23.274	3441	3449	3456	rBV2	3980579	7678755	82.20%	7.236%
42	23.333	3456	3459	3465	rVV	259762	409496	4.38%	0.386%
43	23.410	3465	3472	3487	rVV2	2413146	4785290	51.23%	4.509%
44	23.963	3561	3566	3572	rVB	219649	384945	4.12%	0.363%
45	24.686	3684	3689	3696	rVB2	193996	380364	4.07%	0.358%


Sum of corrected areas: 106119219

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN050119\
Data File : BN005404.D
Acq On : 01 May 2019 11:19
Operator : JU/SJ
Sample : PB119345BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

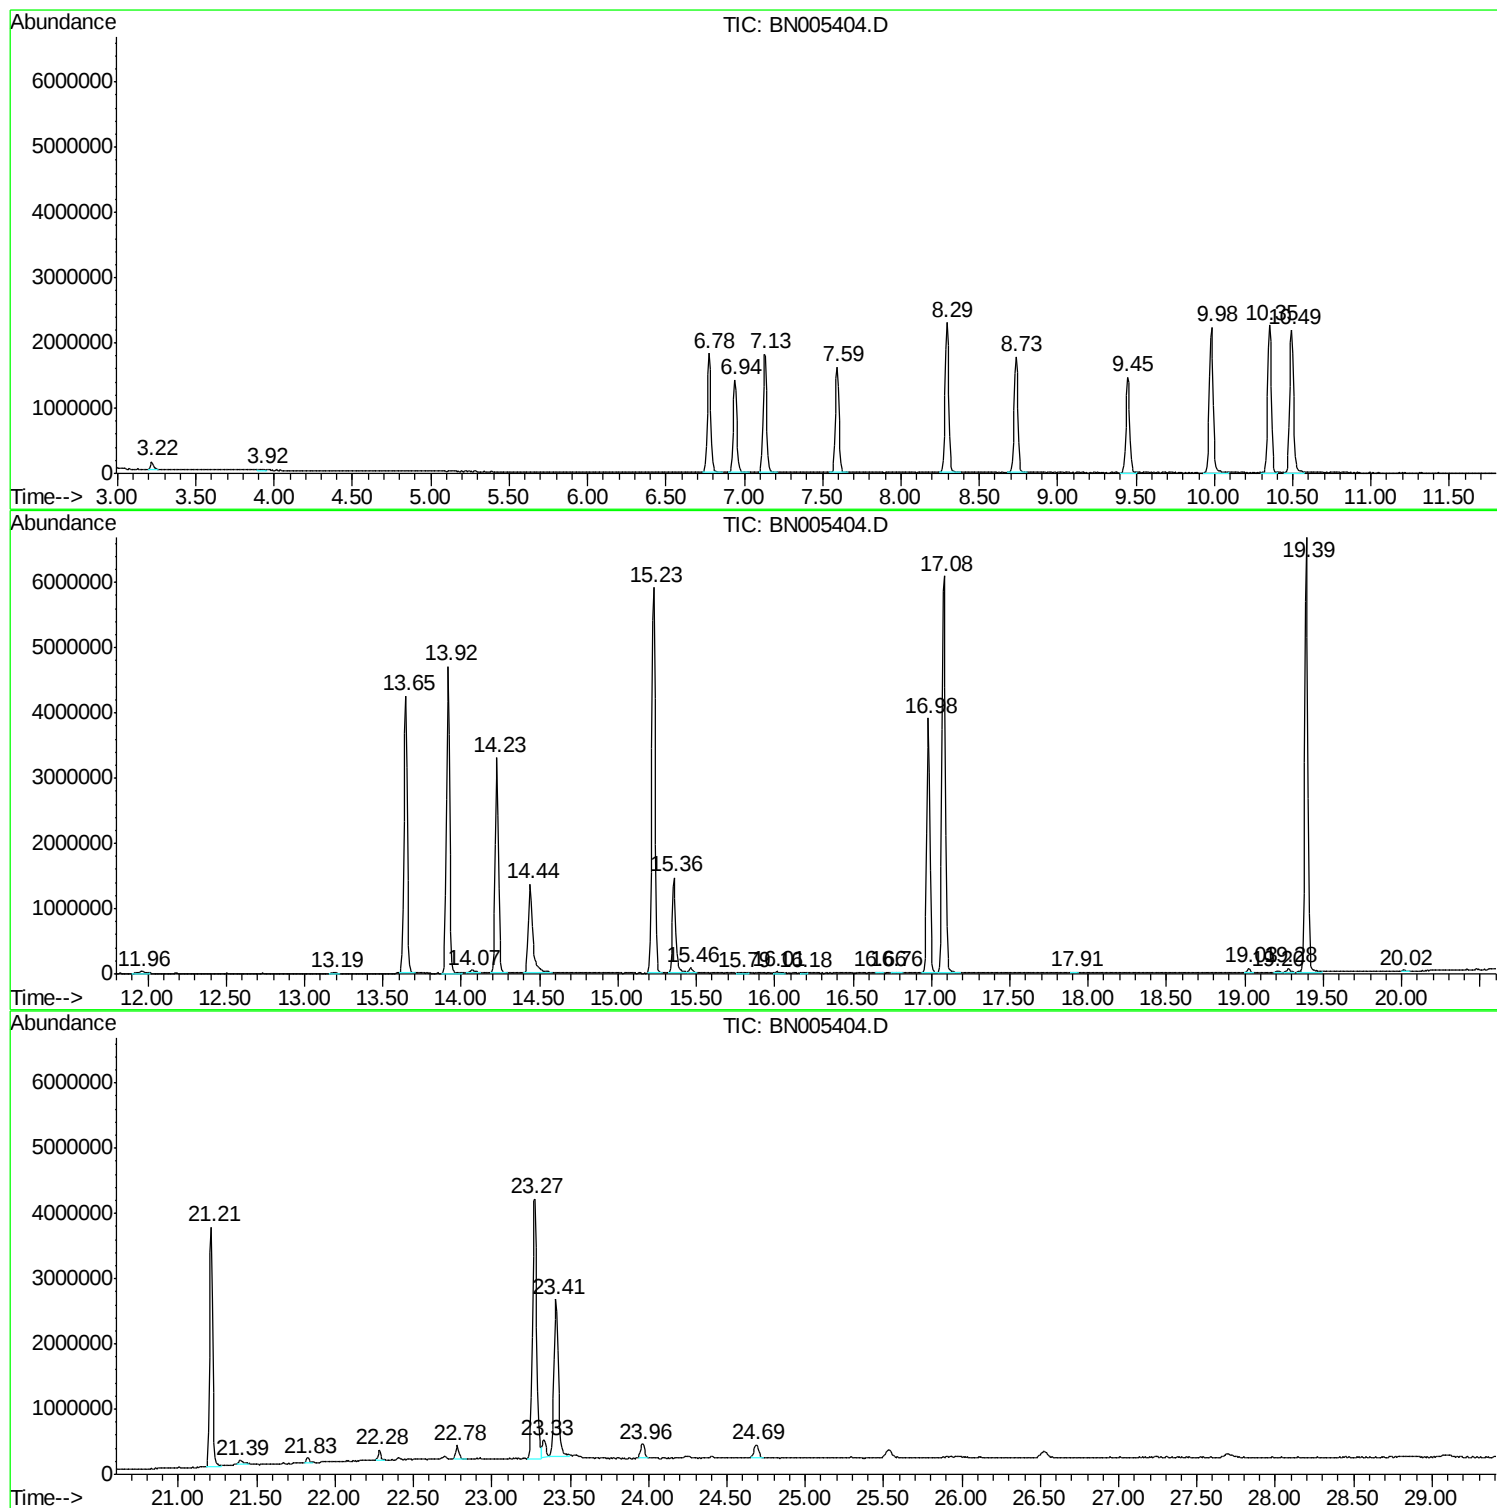

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050119\
Data File : BN005404.D
Acq On : 01 May 2019 11:19
Operator : JU/SJ
Sample : PB119345BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN050119\
Data File : BN005404.D
Acq On : 01 May 2019 11:19
Operator : JU/SJ
Sample : PB119345BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK45

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN041919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc