

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
 Data File : BN031366.D
 Acq On : 02 May 2024 03:08
 Operator : MA/JU
 Sample : P2119-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE6

Quant Time: May 02 03:58:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 02 00:07:34 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.610	152	125173	20.000	ng/u1	0.00
20) Naphthalene-d8	10.393	136	641026	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.257	164	429138	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.010	188	844215	20.000	ng/u1	0.00
79) Chrysene-d12	21.245	240	689629	20.000	ng/u1	-0.01
88) Perylene-d12	24.133	264	887525	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	17858	6.642	ng/uL	0.00
4) Pyridine-d5	3.540	84	227439	29.541	ng/u1	0.00
7) Phenol-d5	6.787	99	301735	29.956	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.957	67	175915	29.828	ng/u1	0.00
11) 2-Chlorophenol-d4	7.146	132	249266	30.933	ng/u1	0.00
15) 4-Methylphenol-d8	8.316	113	268575	32.176	ng/u1	0.00
21) Nitrobenzene-d5	8.769	128	144178	31.209	ng/u1	0.00
24) 2-Nitrophenol-d4	9.481	143	157362	31.649	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.016	165	279890	30.314	ng/u1	0.00
31) 4-Chloroaniline-d4	10.534	131	234318	17.512	ng/u1	0.00
46) Dimethylphthalate-d6	13.675	166	822779	29.082	ng/u1	0.00
49) Acenaphthylene-d8	13.951	160	969101	29.522	ng/u1	0.00
54) 4-Nitrophenol-d4	14.481	143	117725	22.929	ng/u1	0.00
60) Fluorene-d10	15.257	176	477372	19.759	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	49498	11.402	ng/u1	0.00
73) Anthracene-d10	17.110	188	1062616	30.499	ng/u1	0.00
81) Pyrene-d10	19.416	212	1106846	26.353	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.939	264	1242667	30.243	ng/u1	0.00
Target Compounds						
18) 4-Methylphenol	8.375	108	107479	12.351	ng/u1	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
Data File : BN031366.D
Acq On : 02 May 2024 03:08
Operator : MA/JU
Sample : P2119-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE6

Quant Time: May 02 03:58:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 02 00:07:34 2024
Response via : Initial Calibration

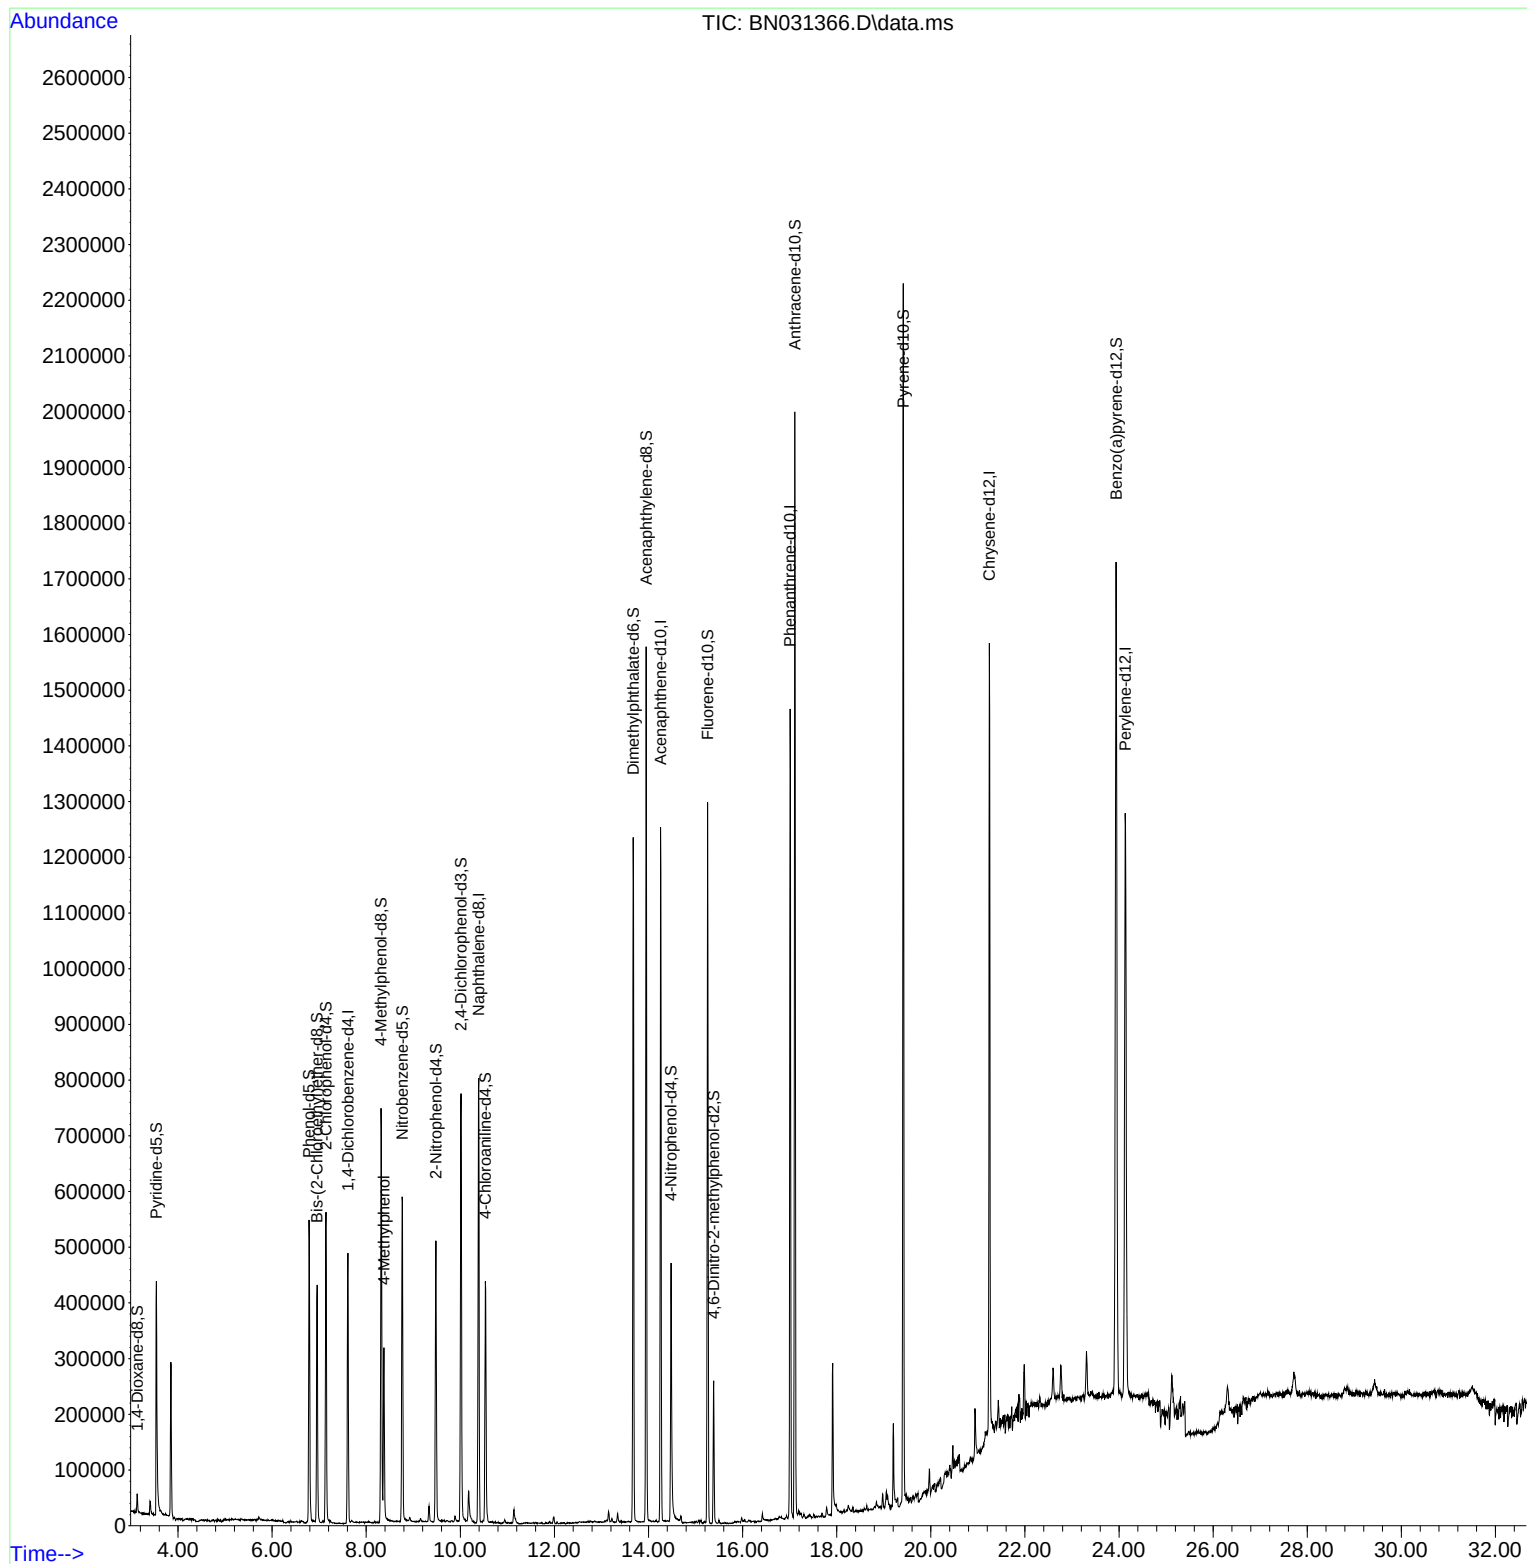

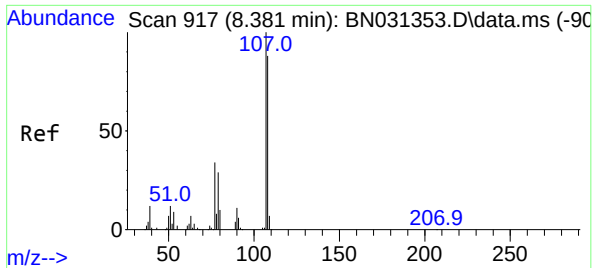

#18
4-Methylphenol
Concen: 12.351 ng/ul
RT: 8.375 min Scan# 91
Delta R.T. -0.006 min
Lab File: BN031366.D
Acq: 02 May 2024 03:08

Instrument :
BNA_N
ClientSampleId :
C0AE6

Tgt Ion:108 Resp: 107479
Ion Ratio Lower Upper
108 100
107 124.6 86.4 129.6

