

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
 Data File : BN031348.D
 Acq On : 01 May 2024 13:38
 Operator : MA/JU
 Sample : PB160361BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK361

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN031348.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	21	25	34	rVB	47163	64129	1.71%	0.167%
2	3.540	92	94	111	rBV	285257	471885	12.60%	1.231%
3	3.852	144	147	151	rVB	10844	13055	0.35%	0.034%
4	4.928	325	330	337	rBV4	8270	20005	0.53%	0.052%
5	6.734	634	637	640	rBV4	2585	3854	0.10%	0.010%
6	6.787	640	646	660	rVV	626831	1017558	27.18%	2.654%
7	6.958	668	675	689	rVB	525802	824976	22.03%	2.151%
8	7.146	700	707	718	rBV	673543	1061734	28.36%	2.769%
9	7.610	779	786	797	rBV	653551	1025562	27.39%	2.675%
10	8.316	899	906	919	rBV	747467	1260676	33.67%	3.288%
11	8.769	976	983	995	rBV	594100	979693	26.16%	2.555%
12	9.481	1097	1104	1117	rBV	509772	834730	22.29%	2.177%
13	10.016	1188	1195	1214	rBV	737871	1262641	33.72%	3.293%
14	10.175	1217	1222	1225	rVB7	2319	3834	0.10%	0.010%
15	10.387	1251	1258	1267	rBV	815915	1371207	36.62%	3.576%
16	10.540	1279	1284	1291	rBV5	5278	10739	0.29%	0.028%
17	11.987	1524	1530	1534	rBV2	12826	20964	0.56%	0.055%
18	13.151	1724	1728	1736	rBV5	8327	14939	0.40%	0.039%
19	13.675	1811	1817	1829	rBV	1301370	1847628	49.34%	4.818%
20	13.951	1856	1864	1877	rBV	1411671	2053218	54.83%	5.354%
21	14.257	1910	1916	1930	rVB	1187473	1755434	46.88%	4.578%
22	14.387	1934	1938	1942	rVB6	2875	4901	0.13%	0.013%
23	14.475	1945	1953	1973	rBV	576518	1008888	26.94%	2.631%
24	14.687	1987	1989	1996	rVB8	4237	7771	0.21%	0.020%
25	14.904	2020	2026	2032	rBV7	4939	9121	0.24%	0.024%
26	15.257	2079	2086	2096	rBV	1924465	2662343	71.10%	6.943%
27	15.386	2102	2108	2121	rBV	619754	868629	23.20%	2.265%
28	15.498	2123	2127	2131	rVB5	8417	11870	0.32%	0.031%
29	15.769	2169	2173	2179	rBV	17127	23076	0.62%	0.060%
30	16.039	2214	2219	2223	rBV6	6937	11010	0.29%	0.029%
31	16.798	2346	2348	2353	rBV5	3353	4672	0.12%	0.012%
32	17.010	2378	2384	2395	rBV	1437274	2054655	54.87%	5.358%
33	17.110	2395	2401	2414	rBV2	2065623	2958527	79.01%	7.715%
34	17.692	2493	2500	2505	rBV2	32714	43750	1.17%	0.114%
35	17.786	2512	2516	2517	rBV3	3733	4446	0.12%	0.012%
36	17.910	2532	2537	2547	rBV	94680	166778	4.45%	0.435%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
Data File : BN031348.D
Acq On : 01 May 2024 13:38
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Title : SVOA CALIBRATION

37	18.980	2715	2719	2721	rBV2	26024	33060	0.88%	0.086%
38	19.010	2721	2724	2728	rVV2	29206	31887	0.85%	0.083%
39	19.051	2728	2731	2736	rVV	22591	31135	0.83%	0.081%
40	19.204	2754	2757	2764	rBV	78470	113425	3.03%	0.296%
41	19.357	2780	2783	2787	rVB4	14196	17027	0.45%	0.044%
42	19.416	2787	2793	2802	rBV	2651539	3532174	94.33%	9.211%
43	21.251	3100	3105	3113	rBV2	1688045	2303367	61.51%	6.007%
44	23.951	3555	3564	3580	rVB2	1464241	3744422	100.00%	9.765%
45	24.145	3589	3597	3609	rVB2	1144722	2780269	74.25%	7.251%




Sum of corrected areas: 38345664

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
Data File : BN031348.D
Acq On : 01 May 2024 13:38
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

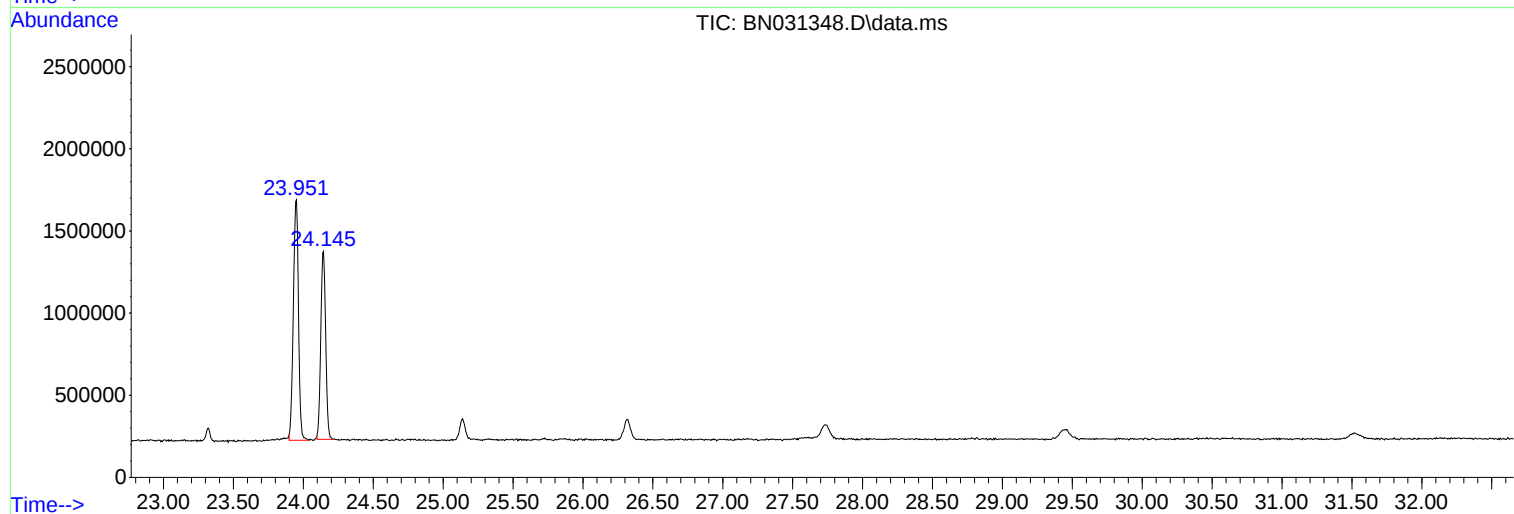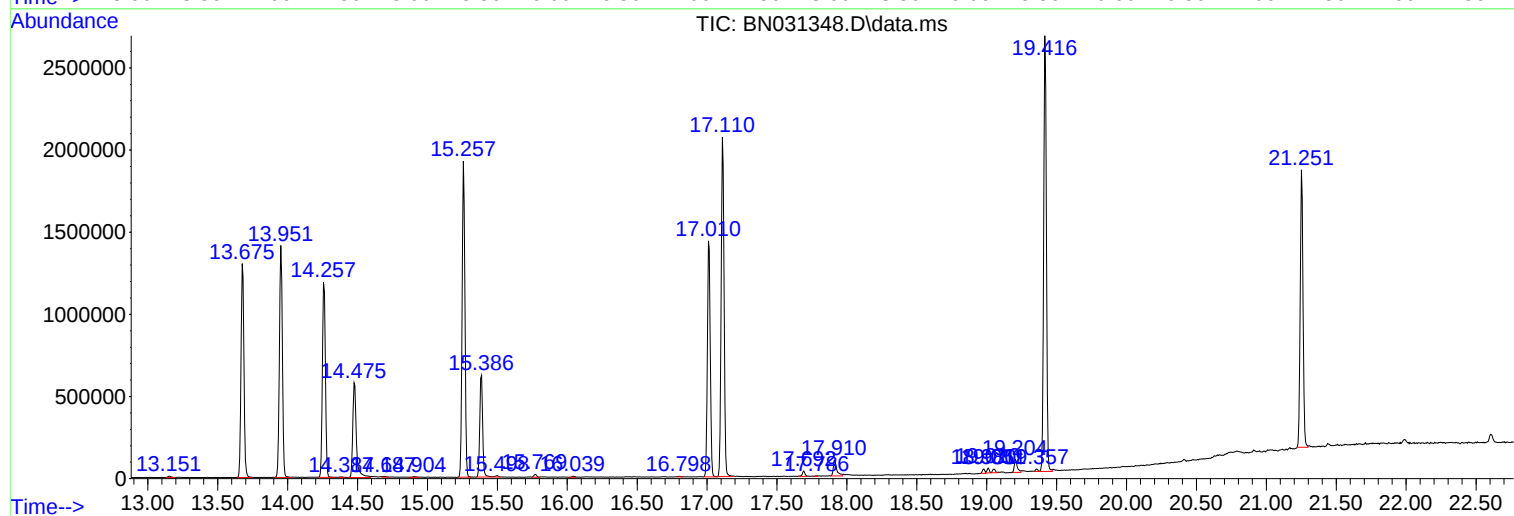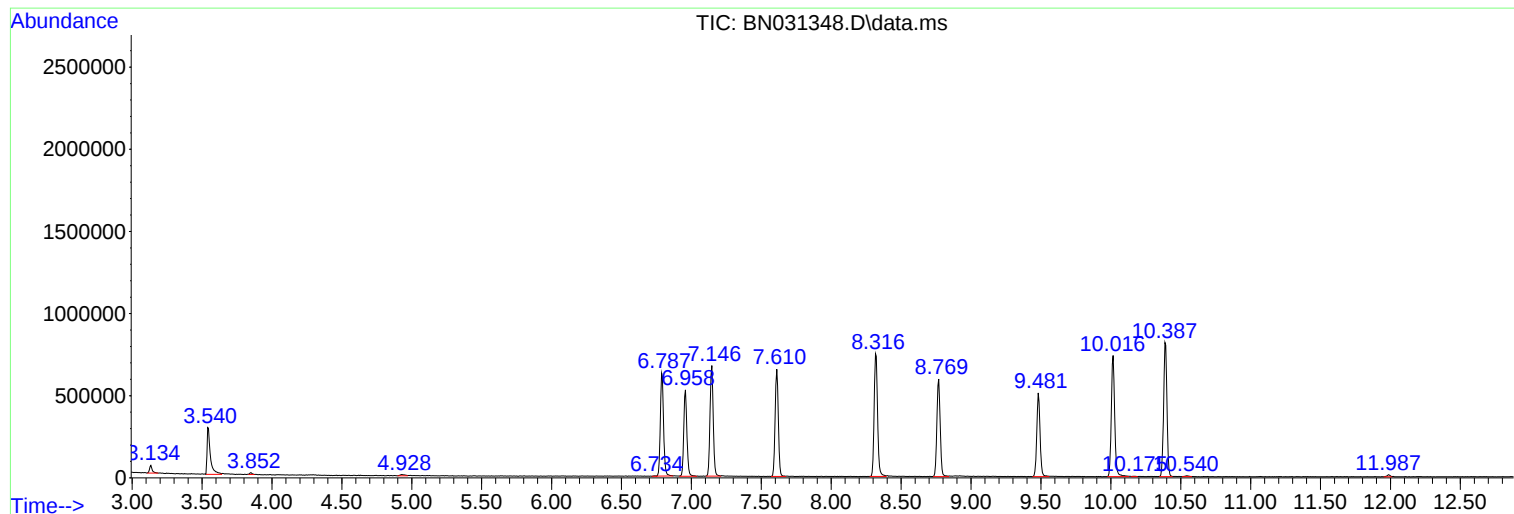

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
Data File : BN031348.D
Acq On : 01 May 2024 13:38
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN050124\
Data File : BN031348.D
Acq On : 01 May 2024 13:38
Operator : MA/JU
Sample : PB160361BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK361

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN042924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------