

#2

1,4-Dioxane

Concen: 7.079 ng/uL

RT: 3.25 min Scan# 44

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA\_N

ClientSampleId :


Tgt Ion: 88 Resp: 42019

Ion Ratio Lower Upper




88 100

43 29.1 25.3 37.9

58 78.5 62.3 93.5

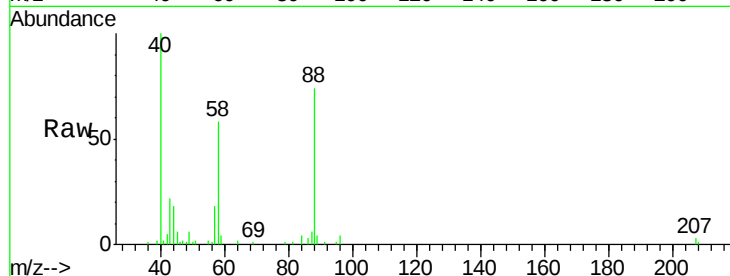

Abundance Ion 88.00 (87.70 to 88.70): BN0  
Ion 43.00 (42.70 to 43.70): BN0  
Ion 58.00 (57.70 to 58.70): BN0

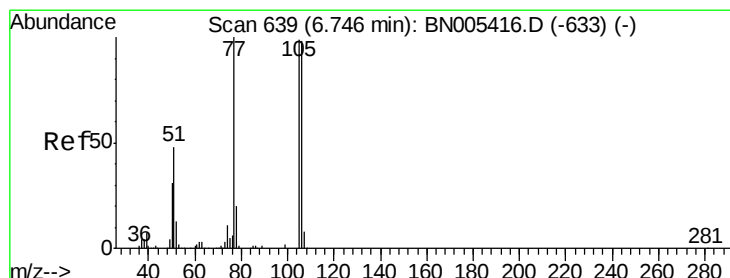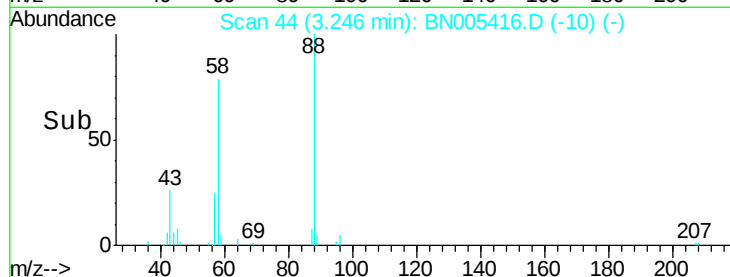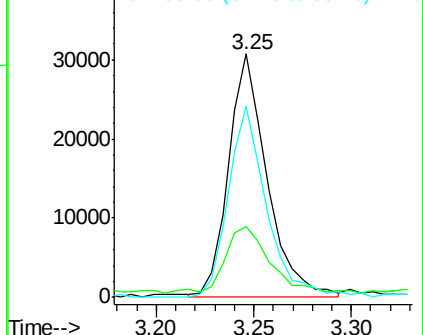

#4

Benzaldehyde

Concen: 18.855 ng/uL

RT: 6.75 min Scan# 639

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34


Tgt Ion: 77 Resp: 279639

Ion Ratio Lower Upper

77 100

105 99.4 77.4 116.2

106 97.6 76.3 114.5

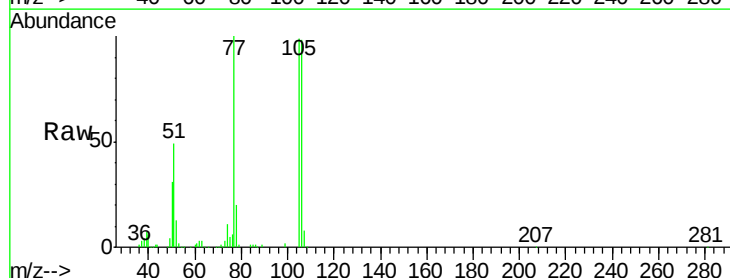

Abundance Ion 77.00 (76.70 to 77.70): BN0  
Ion 105.00 (104.70 to 105.70): BN0  
Ion 106.00 (105.70 to 106.70): BN0

