

#10

2-Chlorophenol

Concen: 20.138 ng/ul

RT: 7.16 min Scan# 710

Delta R.T. 0.00 min

Lab File: BN005416.D

Acq: 02 May 2019 15:34

Instrument :

BNA_N

ClientSampled :


Tgt Ion:128 Resp: 333455

Ion Ratio Lower Upper

128 100

64 48.3 42.3 63.5




130 32.1 26.5 39.7

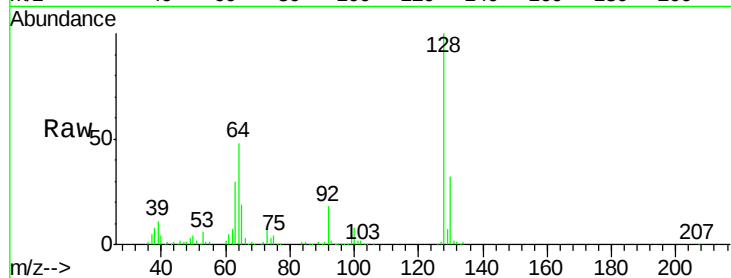

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BNO

Ion 130.00 (129.70 to 130.70): E

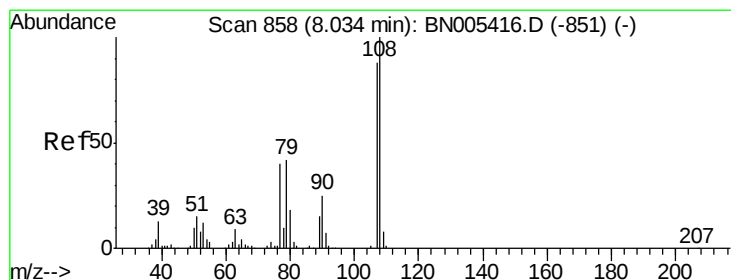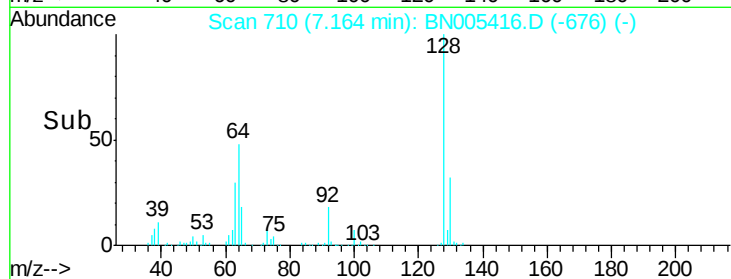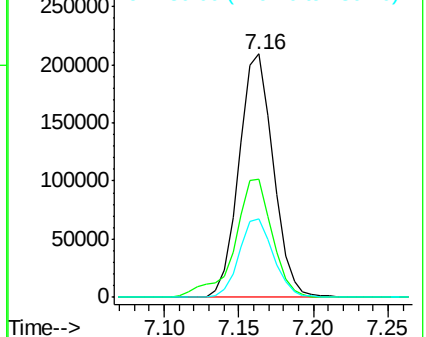

#11

2-Methylphenol

Concen: 20.010 ng/ul

RT: 8.03 min Scan# 858

Delta R.T. 0.00 min

Lab File: BN005416.D


Acq: 02 May 2019 15:34

Tgt Ion:108 Resp: 322775

Ion Ratio Lower Upper

108 100

107 87.9 72.9 109.3

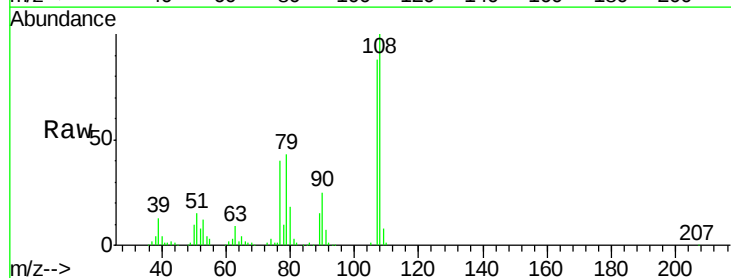

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

